


A new corrosion method (Aycan's method)

Kenan Aycan¹, Fatma Köse², Burcu Kamaşak Arpaçay¹, Tufan Ulçay¹, Ayhan Düzler³

¹Department of Anatomy, Faculty of Medicine, Kırşehir Ahi Evran University, Kırşehir, Türkiye

²Department of Veterinary Anatomy, Institute of Health Sciences, Erciyes University, Kayseri, Türkiye

³Department of Anatomy, Veterinary Faculty, Erciyes University, Kayseri, Türkiye

[Received: 23 April 2024; Accepted: 9 June 2024; Early publication date: 11 June 2024]

Background: As it is known, the anatomy of the vessels is examined by removing the cast of the vessels inside the organs. Generally, liquid material (polyester, takilon, etc.) is injected into the vessels with positive pressure to remove the cast from the vessels of the organs. We built a machine to remove the cast of the vessels inside the organ. We named it corrosion machine.

Materials and methods: Sheep kidneys were used in our experiment. After the kidneys were cannulated, they were placed in the vacuum chamber. With the operation of the vacuum pump, negative pressure was created in the vacuum chamber. With negative pressure, kidneys and its vessels expanded. Takilon or polyester easily entered the vessels of the kidney. The cast of the vessels of the kidney was removed. With this newly developed technique, the anatomy of the vessels whose casts were removed was examined with the naked eye, stereomicroscope or SEM.

Results: The corrosion machine we built can cast the vessels of the organs very well. Takilon or polyester (which we used in our experiment) easily entered the capillaries under the effect of negative pressure.

Conclusions: We think that this method can also be applied to other organs and used in vascular research. (Folia Morphol 2025; 84, 1: 249–255)

Keywords: corrosion, casting method, takilon, polyester, kidney

INTRODUCTION

The distribution of vessels within organs or the internal structure of organs has been investigated by anatomists for years. For this purpose, radiological methods or plastic injection corrosion methods are used [1–3, 5–19]. In the corrosion method, liquid solutions of substances with solidification properties (polyester, nylon, latex, polyvinyl chloride or Mercox CL-2R, methyl methacrylate, vinyl resin) are prepared [1, 7, 11, 14, 19]. The prepared solution is injected into the vessels of the organs using a syringe or other tools. After these liquid substances solidify in the vessels of the organ, the parenchyma of the organ

is melted and the vessels are moulded. The removed mould is examined with the naked eye, stereomicroscope or scanning electron microscopic (SEM). This method is called the corrosion method. With this method, the anatomy of the circulation within the organs is examined [1–3, 5–19]. The corrosion method has been used for years. In this study, liquid substance was injected into the vessels of the organs under negative pressure (vacuum) with the corrosion machine we newly developed, instead of the syringe. With this machine, the cast of the kidney vessels and glomeruli was shown. The features of the method we use are discussed in the light of literature knowledge.

Address for correspondence: Kenan Aycan, Department of Anatomy, Faculty of Medicine, Kırşehir Ahi Evran University, Kırşehir, Türkiye; e-mail: brc1608@gmail.com

This article is available in open access under Creative Common Attribution-Non-Commercial-No Derivatives 4.0 International (CC BY-NC-ND 4.0) license, allowing to download articles and share them with others as long as they credit the authors and the publisher, but without permission to change them in any way or use them commercially.

MATERIALS AND METHODS

We made a machine to use in this experiment (Fig. 1, 2). We named it the corrosion machine. It is separated in two main parts: the vacuum pump (Fig. 1/1) and the glass jar (Figure 1/8). The vacuum pump reduces air pressure in the glass jar. The glass jar allows corrosion fluid to enter the vessels of the organs at low pressure. The other part of the corrosion machine are: an air valve for shut or open the air (Fig. 1/2), a vacuum manometer that shows the vacuum in the glass jar (Fig. 1/3), a corrosion liquid chamber (Fig. 1/4) that contains the corrosion liquid, and a vacuum stabilizer (Fig. 1/5) that organizes the vacuum.

Twenty kidneys from 10 adult Akkaraman sheep (12–20 months old and 35–45 kg) were used in this study. Akkaraman sheep were preferred because they are the most common sheep breed in Türkiye. No live animals were used in the research for this study. The materials were taken from the slaughterhouse and prepared for research. The volumes of the kidneys were measured according to Archimedes' principles [13]. The average volume of the kidneys was determined to be 60 cc. It was decided to give 10 cc of corrosion fluid to each kidney. When the kidneys were taken from the sheep in the slaughterhouse, we started working immediately. The renal arteries of the kidneys were catheterized. The kidneys were placed in a glass jar (Fig. 1).

Takilon (Ece Boya Kimya Sanayi ve Ticaret A.Ş. İstanbul/Türkiye) was used in 10 of the kidneys to remove the caste of the vessels. Corrosion liquid was prepared by mixing 40 g of takilon (monomethylmetacrylate) powder (polymethylmethacrylate) and

1 g of Oil Red. The prepared solution was placed in the corrosion liquid chamber. Vacuum was adjusted to 20 cm Hg Vac with the vacuum stabilizer in the vacuum room (Fig. 1/7). The air valve was closed. The vacuum pump was started. The kidney and its vessels began to expand due to the negative pressure created in the glass jar. The takilon solution in the corrosion fluid chamber filled the intrarenal arteries of the kidney. 10 cc of corrosion fluid was given to each kidney. Negative pressure was terminated by opening the air valve. The vacuum motor was stopped.

Polyester resin (Ece Boya Kimya Sanayi ve Ticaret A.Ş. İstanbul/Türkiye) was used in 10 of the kidneys to remove the caste of the renal vessels. The polyester solution was prepared by adding 100 cc of polyester resin, 2 g of paint, 1 cc of accelerant and 2 cc of catalyst. The prepared solution was placed in the corrosion liquid chamber. The vacuum was adjusted to 20 cm Hg Vac with the vacuum stabilizer. The air valve is closed. The vacuum pump was started. The kidney and its vessels began to expand due to the negative pressure created in the glass jar. The polyester solution in the corrosion fluid chamber filled the intrarenal arteries of the kidney. 10 cc of the polyester solution was given to each kidney. Negative pressure was terminated by opening the air valve. The vacuum motor was stopped.

The prepared kidneys were kept at room temperature for 24 hours for polymerization to occur. The polymerized takilon kidneys were kept in an oven in 20% KOH solution at 37°C for 24 hours. The kidneys were washed in tap water and the vessel cast was removed. The polymerized polyester kidneys were placed in hydrochloric acid (HCL) and kept for 24 hours. The kidneys were washed in tap water and the vessel cast was removed. Photographs of the

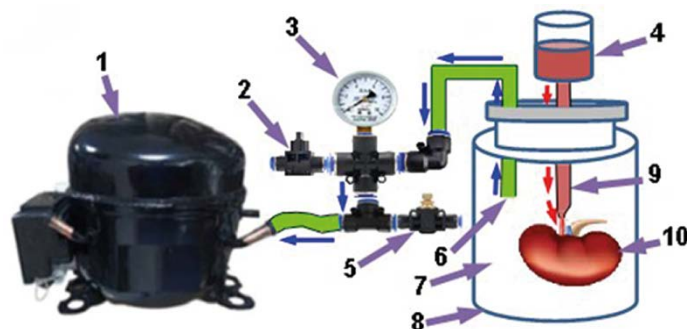


Figure 1. Corrosion machine. Vacuum pump (1), air valve (2), manometers of vacuum (3), corrosion liquid chamber (4), vacuum stabilizer (5), air discharge pipe (6), vacuum room, negative pressure (7), glass jar (vacuum chamber) (8), corrosion liquid pipe (9), kidney (10).

removed casts were taken. Capillaries were examined both by stereo microscope (Olympus SZX16) and scanning electron microscope (SEM, Zeiss gemini 500) [1].

RESULTS

In our study, we removed the cast of the renal arteries with the method we newly developed (Fig. 3–6). We used the corrosion machine we developed in our study (Fig. 1, 2). When the corrosion machine worked, it created negative pressure in a closed container (glass jar). The negative pressure in the jar expanded the kidneys and their vessels. As a result of the negative pressure, corrosion fluid (takilon or polyester) easily entered the capillaries of the kidney. We used takilon (Fig. 3, 6, 7) and polyester (Fig. 4, 5) as corrosion fluid with the corrosion machine.

In our study, we used easily available sheep kidneys. We removed the cast of the kidney vessels with our corrosion machine. With this method, we examined the renal arteries and glomeruli with both a stereomicroscope (Fig. 6) and a scanning electron microscope (Fig. 7).

If the negative pressure is high (20 cm Hg Vac), the anatomy of the capillaries is disrupted, the corrosion fluid fills the kidney parenchyma and the vessel cast is not removed (Fig. 4). The vacuum level can be adjusted with the vacuum stabilizer of the machine. As a result of our experiments, we determined that it is appropriate to adjust the vacuum stabilizer to a maximum of 20 cm Hg Vac. Adjusting the pressure of the corrosion fluid with the corrosion machine we developed is under the control of the researcher.

Before the experiment started, we determined that the average volume of the kidneys was 60 cc by measuring them according to the Archimedes principle. We conducted experiments by giving different amounts of corrosion fluid to the kidneys. As a result of our experiments, we determined that it is appropriate to give 10 cc of corrosion fluid to remove the cast of the renal vessels. If the corrosion fluid given to the kidney is more than 10 cc, the kidney capillaries rupture, the corrosion fluid solidifies in the kidney parenchyma and the vessels are not removed.

With the method we developed, we removed the vessel cast of the kidney and examined its anatomy with the naked eye (Fig. 3–5), and its glomeruli with a stereo microscope and SEM (Fig. 6, 7). The kidney arteries in the casts we removed with this new method were in normal anatomical shape and size.



Figure 2. Corrosion machine.

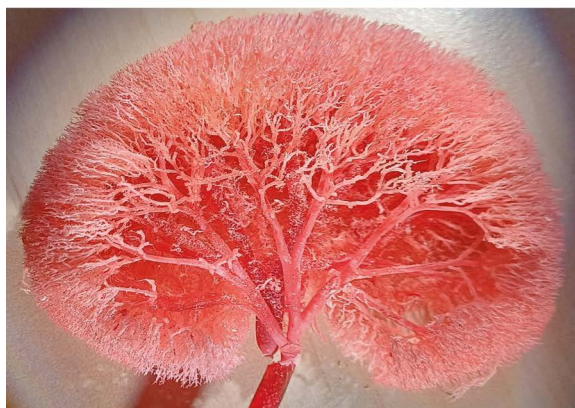
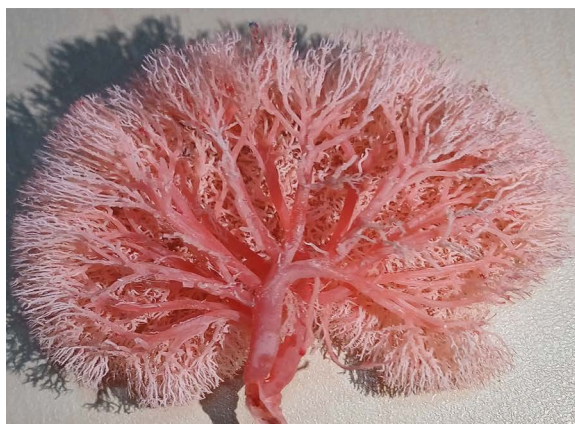


Figure 3. The cast of the sheep kidney vessels with takilon.



Figure 4. Kidney parenchyma filled with corrosion fluid due to high vacuum at different levels and kidneys whose casts cannot be removed.



Figure 5. The cast of the sheep kidney vessels with polyester.

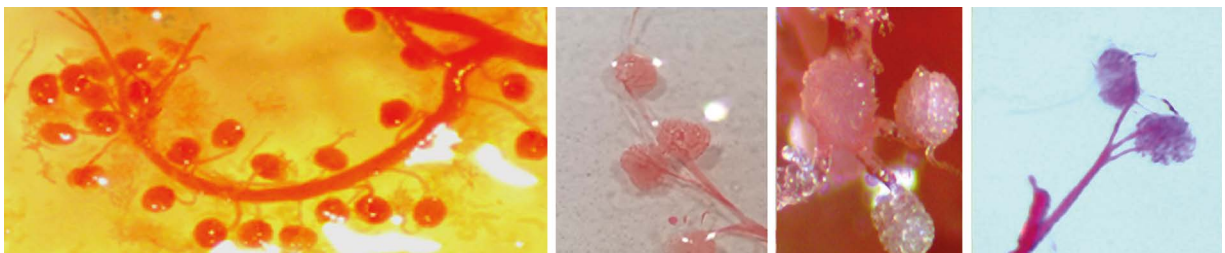


Figure 6. The takilon cast of the glomeruli (stereomicroscopic views).

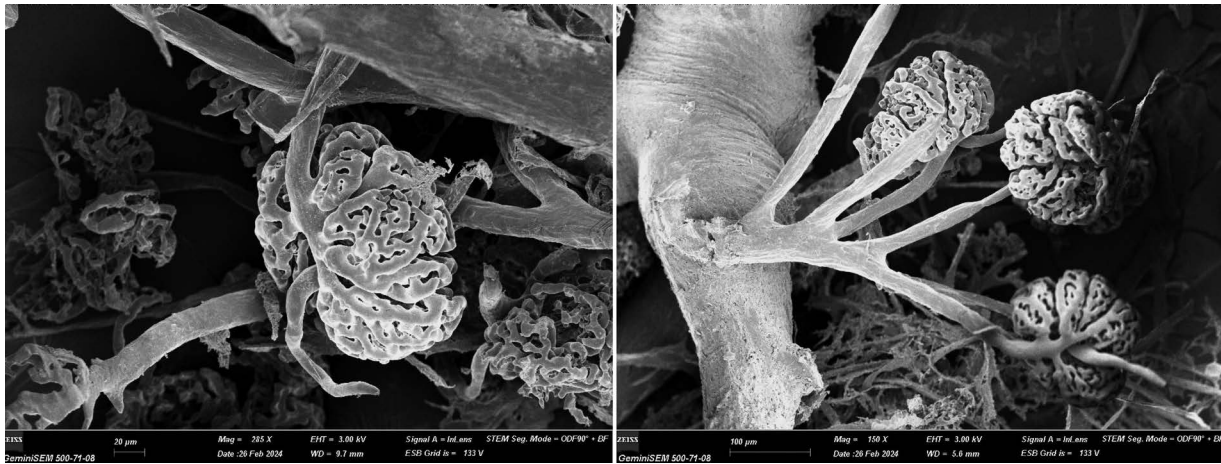


Figure 7. The takilon cast of the glomeruli (scanning electron microscopic).

DISCUSSION

As it is known, the thoracic cavity expands and contracts with the movements of the respiratory muscles. With the negative pressure created in this expansion, air enters the lungs, and in contraction, air leaves the lungs. This event is called inspiration and expiration. Air enters the lungs under the effect of the negative pressure (vacuum) formed in the thoracic cavity [4]. The method we applied was created by making use of the inspiration and expiration mechanism. The working principle of the corrosion machine we developed is to create negative pressure in a closed container (glass jar) so that the corrosion fluid can easily enter the vessels of the organ. As a result of the negative pressure in the glass jar, the organ in the jar and its vessels expand. Corrosion fluid (takilon or polyester) easily enters the capillaries of the organ. The removed casts preserve the normal anatomical shape and size of the vessels.

We used polyester and takilon to demonstrate the feasibility of the method. These chemicals can be easily found on the market in Turkey. Later, we will test whether other chemicals can be used in this method.

In our study, it has been shown that corrosion fluid easily enters the kidney vessels with negative pressure. The cast of the kidney vessels has been removed. We believe that this method can also be applied to other organs.

In known corrosion methods, the prepared corrosion fluid is injected into the vessels of the organs with positive pressure [1–3, 5–19]. In this study, instead of positive pressure, negative pressure was applied to the organs, allowing corrosion fluid to enter the

vessels. As a result of negative pressure, the organ and its vessels expand, and the corrosion fluid easily enters the expanded vessels. It is easier to remove the mould of the vessels by applying vacuum instead of using injection. Our method is important in terms of ease of use. For this purpose, we developed the vacuum corrosion machine.

When the sheep were slaughtered, the kidneys were removed immediately. The method was implemented without any delay. No anticoagulant chemicals (Heparin-acetone-coumarin) were used. As seen in our findings, there was no clotting problem. Removing the cast of the glomeruli shows that there is no clotting problem. According to our findings, we think that negative pressure solves the clotting problem by expanding the vascular lumen. This result showed that the method can be used in corrosion.

If too much corrosion liquid enters the kidney, the capillaries of the kidney rupture, and the corrosion liquid fills the parenchyma of the kidney. The cast of the vessels of the kidney cannot be removed as the corrosion liquid hardens within the parenchyma. The amount of corrosion liquid administered to the kidney should only fill the vessels. For this purpose, we calculated the average volume of the kidneys by using Archimedes' principle [13]. We determined that the average volume of the kidneys is 60 cc. As a result of our experiments, we determined that it is appropriate to give 10 cc of corrosion liquid to remove the cast of the renal vessels. If the amount of corrosion liquid given to the kidney is more than 10 cc, it ruptures the capillaries, the

kidney parenchyma hardens, and the blood vessels do not come out. The amount of corrosion liquid is controlled by the indicator in the corrosion liquid chamber. Researchers who use this method must carefully adjust the amount of corrosion liquid to be administered to the organ from which the vessel cast will be removed.

In our experiment, the negative pressure in the glass jar was observed with a vacuum manometer. If the vacuum applied to the organ is high (for example: 40 cm Hg Vac), the kidney capillaries rupture and cast is not removed. In our study, it was determined that the appropriate vacuum applied should be around 10–20 cm Hg Vac. The pressure to be applied during the experiment can be adjusted by opening the air valve. More or less negative pressure affects the result of the experiment. Thus, we believe that this method we have developed can be used in anatomy education to examine the anatomy of the vessels of organs.

CONCLUSIONS

In the corrosion machine we have developed, takilon and polyester can be used as corrosion liquids if desired. With these substances, the cast of the vessels can be removed. We believe that other corrosion materials (latex, polyurethane, nylon, etc.) can also be used with this machine.

Summing up, the corrosion machine we built can cast the vessels of the organs very well. Polyester or takilon can be used to remove the cast of the vessels of organs with the corrosion machine, and we believe that other materials can also be used. We think that if a large vacuum chamber is built instead of the jar, the vessels and the other cavities of larger organs (liver, lung, etc.) can be cast. We believe that this method may be useful for those who want to remove the cast of the cavities.

ARTICLE INFORMATION AND DECLARATIONS

Data availability statement

The data that support the findings of this study are available on request from the corresponding author.

Ethics statement

This study was conducted on sheep cadaver kidneys and is among the studies that do not require ethics committee approval.

Acknowledgments

We would like to thank the faculty members of the Department of Anatomy, Faculty of Medicine, Kırşehir Ahi Evran University and Department of Veterinary Anatomy, Faculty of Veterinary Medicine, Erciyes University.

Author contributions

Kenan Aycan: Preparation of the study, data collection and analysis, writing & editing. Fatma Köse: Data collection. Burcu Kamaşak Arpaçay: Data collection, Writing & editing. Tufan Ulcay: Data analysis. Ayhan Düzler: Data analysis and supervision.

Funding

No funding.

Conflict of interest

The authors declare no conflict of interest.

REFERENCES

1. Aycan K, Ulcay T, Kamaşak B. The morphology of the afferent and efferent domain of the sheep glomerulus. *Folia Morphol.* 2021; 80(4): 881–887, doi: [10.5603/FM.a2020.0124](https://doi.org/10.5603/FM.a2020.0124), indexed in Pubmed: [33084008](https://pubmed.ncbi.nlm.nih.gov/33084008/).
2. Aydinlik E, Aycan K, Ekinci N. Anatomy of the coronary veins in akkaraman sheep. *J Health Sci.* 2000; 17(1): 40–45.
3. Bordei P, St Antohe D, Sapte E, et al. Morphological aspects of the inferior suprarenal artery. *Surg Radiol Anat.* 2003; 25(3-4): 247–251, doi: [10.1007/s00276-003-0132-z](https://doi.org/10.1007/s00276-003-0132-z), indexed in Pubmed: [14504822](https://pubmed.ncbi.nlm.nih.gov/14504822/).
4. Boron WF. Organisation of the Respiratory System. In: Boron WF, Boulpaep EL. ed. *Medical Physiology*. 3rd ed. Elsevier: 590–700.
5. Brown JA. Renal microvasculature of the rainbow trout, *Salmo gairdneri*: scanning electron microscopy of corrosion casts of glomeruli. *Anat Rec.* 1985; 213(4): 505–513, doi: [10.1002/ar.1092130405](https://doi.org/10.1002/ar.1092130405), indexed in Pubmed: [4083531](https://pubmed.ncbi.nlm.nih.gov/4083531/).
6. Casotti G, Braun EJ. Structure of the glomerular capillaries of the domestic chicken and desert quail. *J Morphol.* 1995; 224(1): 57–63, doi: [10.1002/jmor.1052240107](https://doi.org/10.1002/jmor.1052240107), indexed in Pubmed: [7723047](https://pubmed.ncbi.nlm.nih.gov/7723047/).
7. De Sordi N, Bombardi C, Chiocchetti R, et al. A new method of producing casts for anatomical studies. *Anat Sci Int.* 2014; 89(4): 255–265, doi: [10.1007/s12565-014-0240-3](https://doi.org/10.1007/s12565-014-0240-3), indexed in Pubmed: [24788383](https://pubmed.ncbi.nlm.nih.gov/24788383/).
8. Domagała Z, Domański J, Smyczek N, et al. Maceration stage in corrosion cast specimen procedure in anatomy: a minireview. *Folia Morphol.* 2022; 81(4): 825–833, doi: [10.5603/FM.a2021.0119](https://doi.org/10.5603/FM.a2021.0119), indexed in Pubmed: [34750800](https://pubmed.ncbi.nlm.nih.gov/34750800/).
9. Düzler A, Nur İH, Alan AA. Macroanatomical study on ramification and course of aorta descendens in japanese quail. *J Fac Vet Med Univ.* 2011; 8(3): 139–152.
10. Elger M, Sakai T, Kriz W. The vascular pole of the renal glomerulus of rat. *Adv Anat Embryol Cell Biol.* 1998; 139: 1–98, doi: [10.1007/978-3-642-80449-6](https://doi.org/10.1007/978-3-642-80449-6).

11. Ilić M, Milisavljević M, Maliković A, et al. The superficial palmar branch of the radial artery: a corrosion cast study. *Folia Morphol.* 2018; 77(4): 649–655, doi: [10.5603/FM.a2018.0033](https://doi.org/10.5603/FM.a2018.0033), indexed in Pubmed: [29611162](https://pubmed.ncbi.nlm.nih.gov/29611162/).
12. Kłosińska D, Ciszek B, Majchrzak B, et al. Diversity of coronary arterial tree in laboratory mice. *Folia Morphol.* 2020; 79(2): 255–264, doi: [10.5603/FM.a2019.0070](https://doi.org/10.5603/FM.a2019.0070), indexed in Pubmed: [31257564](https://pubmed.ncbi.nlm.nih.gov/31257564/).
13. Kose F, Duzler A. An anatomical and volumetric study on brain ventricles in sheep using different techniques. *Anat Histol Embryol.* 2023; 52(5): 732–741, doi: [10.1111/ahe.12930](https://doi.org/10.1111/ahe.12930), indexed in Pubmed: [37165795](https://pubmed.ncbi.nlm.nih.gov/37165795/).
14. Maga P, Tomaszewski KA, Skrzat J, et al. Microanatomical study of the recurrent artery of Heubner. *Ann Anat.* 2013; 195(4): 342–350, doi: [10.1016/j.aanat.2013.03.011](https://doi.org/10.1016/j.aanat.2013.03.011), indexed in Pubmed: [23701902](https://pubmed.ncbi.nlm.nih.gov/23701902/).
15. Narayanan VR. Preparation of low cost bronchopulmonary airway cast. *J Anat Soc India.* 2015; 64(2): 162–165, doi: [10.1016/j.jasi.2015.10.007](https://doi.org/10.1016/j.jasi.2015.10.007).
16. Nerantzis C, Antonakis E, Avgoustakis D. A new corrosion casting technique. *Anat Rec.* 1978; 191(3): 321–325, doi: [10.1002/ar.1091910305](https://doi.org/10.1002/ar.1091910305), indexed in Pubmed: [354429](https://pubmed.ncbi.nlm.nih.gov/354429/).
17. Oguz O, Dere F, Yücel AH, et al. Examination of microvascular structures of midcortical region in sheep kidneys: a three dimensional approach. *Acta Med Okayama.* 1991; 45(2): 77–80, doi: [10.18926/AMO/32185](https://doi.org/10.18926/AMO/32185), indexed in Pubmed: [1867114](https://pubmed.ncbi.nlm.nih.gov/1867114/).
18. Oguz O, Dere F, Yücel AH, et al. Scanning electron microscopic (SEM) examination of structures which supply subcapsular and midcortical region postglomerular microcirculation in sheep kidney. *Acta Morphol Hung.* 1992; 40(1-4): 195–202, indexed in Pubmed: [1365763](https://pubmed.ncbi.nlm.nih.gov/1365763/).
19. Shanthini S, Suma HY. An innovative method in venous coronary cast technique. *Anat Cell Biol.* 2019; 52(2): 191–195, doi: [10.5115/acb.2019.52.2.191](https://doi.org/10.5115/acb.2019.52.2.191), indexed in Pubmed: [31338236](https://pubmed.ncbi.nlm.nih.gov/31338236/).