


Available online at [www.sciencedirect.com](http://www.sciencedirect.com)

ScienceDirect

journal homepage: <http://www.elsevier.com/locate/pjnns>

## Case report

# Delayed perforation of posterior pharyngeal wall caused by dislodged bioresorbable interbody cage. Case report

Krzysztof Zapałowicz<sup>a,\*</sup>, Maciej Radek<sup>a</sup>, Maciej Wojdyn<sup>a</sup>, Piotr Pietkiewicz<sup>b</sup>, Jurek Olszewski<sup>b</sup>

<sup>a</sup>Department of Neurosurgery and Peripheral Nerve Surgery, Medical University of Łódź, University Hospital WAM-CSW, Łódź, Poland

<sup>b</sup>Department of Otolaryngology and Laryngological Oncology, Medical University of Łódź, University Hospital WAM-CSW, Łódź, Poland

## ARTICLE INFO

## Article history:

Received 10 June 2013

Accepted 16 December 2013

Available online 23 January 2014

## Keywords:

Anterior cervical fusion

Cervical interbody cage

Biomaterials

Pharyngeal perforation

Complication

## ABSTRACT

A 48-year-old man was admitted for the management of congenital anomalies: Arnold–Chiari type I malformation combined with odontoid upward migration. He also had degenerative stenosis of the spinal canal by spurs at C2/C3 and C3/C4 levels. Osseous deformities caused ischaemic changes of the brainstem as well as spinal cord compression. Authors used the Biocage – interbody cage covered by bioresorbable layer to fill the surgically created gap after removal of the right part of C3 vertebral body. Twenty-seven months after implantation, the implant was extruded through posterior pharyngeal wall. Authors describe this unusual case and discuss possible causes of Biocage extrusion.

© 2014 Polish Neurological Society. Published by Elsevier Urban & Partner Sp. z o.o. All rights reserved.

## 1. Introduction


Historically, the first methods of anterior decompression of the cervical spinal cord used bone grafts as the material for interbody fusion [1,2]. As an alternative way, implantation of cages made of metals or synthetic materials has been proposed instead of bone grafts [1–4]. Bioresorbable implants made of lactic acid polymer were introduced in 1966 to stabilize long-bone fractures, and later were adapted to spinal surgery [3]. Their inherent properties entail gradual resorption in physiological milieu [3–6] and elastic modulus more similar to the bone than that of titanium or nonresorbable polymers

[5,6]. The cervical bioresorbable cage – Biocage (Cousin Biotech) is tubular in shape, and slightly bent to imitate cervical lordosis [7]. The wall of the tube is radiolucent, made of polyester mesh tissue, and impregnated with solution of poly-L-lactic acid (PLLA). The elasticity of both materials reduces the stress-shielding effect. To enable X-ray detection, the longitudinal radiopaque fibre is inserted into the wall [7]. After implantation, the PLLA is gradually resorbed, permitting bone penetration into perforations of the polyester wall [7]. Söderlund et al. implanted Biocage combined with anterior screw-plate system in seventeen patients. After a mean follow-up of thirty months, he concluded that fusion was complete in five cases and probable in ten others, whereas in

\* Corresponding author at: Klinika Neurochirurgii i Chirurgii Nerwów Obwodowych, Uniwersytetu Medycznego w Łodzi, Uniwersytecki Szpital Kliniczny im. WAM-CSW, ul. Żeromskiego 113, 90-549 Łódź, Poland.

E-mail address: [krzysztofzapałowicz1@wp.pl](mailto:krzysztofzapałowicz1@wp.pl) (K. Zapałowicz).

0028-3843/\$ – see front matter © 2014 Polish Neurological Society. Published by Elsevier Urban & Partner Sp. z o.o. All rights reserved.  
<http://dx.doi.org/10.1016/j.pjnns.2014.01.001>

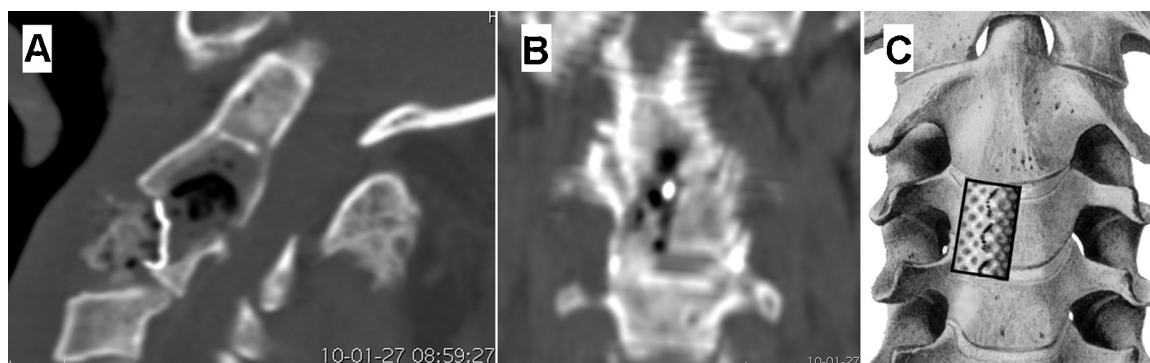

**Fig. 1 – CT of the cervical spine performed two days after Biocage implantation. Sagittal (A) and frontal (B) image reconstructions, with schematic drawing (C), demonstrating the position of Biocage (note the presence of radiopaque fibre).**

two cases the implant did not fuse [7]. Based on encouraging results published by Söderlund et al., we used the Biocage to fill the surgically created gap in the right part of C3 vertebral body. Twenty-seven months after implantation, the Biocage was extruded through posterior pharyngeal wall. We describe this unusual case and discuss possible causes of Biocage extrusion.


## 2. Case report

A 48-year-old man was admitted for management of Arnold–Chiari type I malformation combined with odontoid upward migration. He also had spinal cord compression by spurs at C2/C3 and C3/C4 levels. Osseous deformities caused ischaemic changes of the brainstem as well as spinal cord compression. According to Nurick scale, the patient's neurological status was assessed as grade IV. He underwent consecutive operations: (1) in July 2009 and in October 2010, subtotal odontoidectomies by transpharyngeal approach – during both procedures total removal of the odontoid peg was not successful due to important bleeding; (2) in January 2010, discectomies of C2/C3 and C3/C4 with removal of the right part of the C3 vertebral body, followed by C2–C4 spondylodesis with Biocage (Fig. 1); (3) in May 2010, decompression of the posterior fossa with C1–C4 laminectomies followed by stabilization between occiput and C7. Computed tomography (CT) examinations (April and October 2010) revealed stability of the Biocage (Fig. 2). The patient was reviewed at follow-up examinations demonstrating improvement to Nurick grade


III. In May 2012, he arrived declaring that an odd-looking object had expelled through his mouth during severe cough after two days of dysphagia – in fact it turned out to be a Biocage (Fig. 3). There was no history of trauma or fever. Oropharyngeal examination revealed wound of the posterior pharyngeal wall measuring 1 cm × 2 cm, situated beneath the cicatrised incision used for odontoidectomy (Fig. 4). Complementary investigations showed 4200 leukocytes per mm<sup>3</sup>. Computed tomography disclosed absence of the Biocage in the place of implantation (Fig. 5). Treatment was started by intravenous antibiotics (amoxycillin plus clavulanic acid and metronidazole). The following day the wound was sutured by an otolaryngologic surgeon. The patient was fed by nasogastric tube for nine days. Despite there being no suppuration, the antibiotherapy was continued, combined with Octenidine oral gargles. He was discharged after healing of the wound. Otolaryngologic follow-up revealed cicatrization of the posterior pharyngeal wall.

## 3. Discussion

In order to elucidate the possible cause of Biocage migration, we tried to analyze if this complication might arise from surgical error or other factors. Regarding the surgery, the Biocage was fit to the size of surgically created space between C2 and C4 and tightly placed in its interior. Lack of complementary anterior instrumentation does not explain delayed lack of fusion. Reinforcement of the Biocage by anterior screw-plate system was planned; however, intraoperatively it was ruled out due to

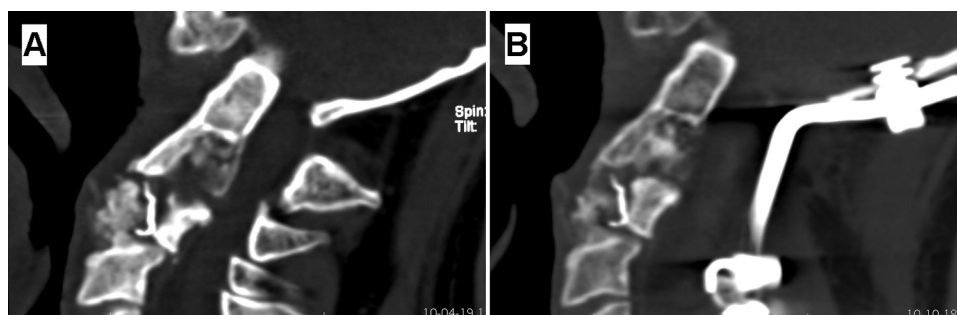

**Fig. 2 – Control CT images performed three months (A) and nine months (B) after implantation. There are no signs of Biocage displacement.**

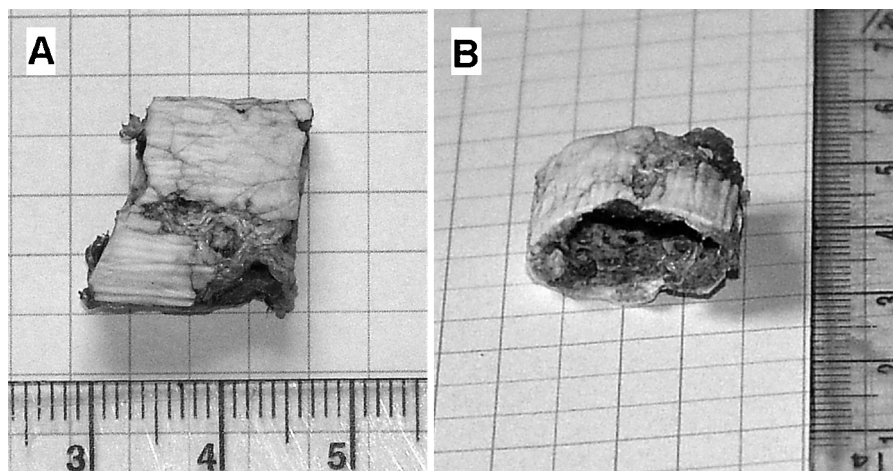

**Fig. 3 – The photographs demonstrating extruded Biocage. (A) The wall of Biocage showing partially uncovered polyester mesh tube and (B) bony material inside the tube. The length of extruded implant is 17–14 mm whereas the transverse cross-section is elliptic with diameters 17 and 8 mm.**


several reasons: limited range of patient's head motion made surgical access to C2 and C3 levels difficult, and two previous transpharyngeal operations had left a scar between posterior pharyngeal wall and C2 vertebra thus denudation of C2 vertebral body for plate screwing carried the risk of pharyngeal perforation. Posterior occipitocervical stabilization took place three

months later. Comparison of CT sagittal reconstructions (Fig. 2), performed before and after occipitocervical instrumentation revealed that position of Biocage did not change, thus manoeuvres associated with posterior surgery can be ruled out as potential mechanism of destabilization. In the light of facts mentioned above, we came up with the following explanation of Biocage migration: the biodegradation of PLLA was not followed by sufficient bone infiltration of remaining polyester mesh. As a consequence, the implant became loose and eroded the posterior pharyngeal wall.

Delayed penetration of the implant used for anterior cervical fusion into oropharynx is considered as a rare complication of such surgery. In majority of cases reported in the literature, the screws from plating systems migrated through pharyngeal or oesophageal wall and were extruded orally or were eliminated through the gastrointestinal tract [8–14]. Fountas et al. [15] in their series of 1015 patients observed 1 case (0.1%) of oesophageal perforation by dislodged screw. Extrusion of larger implant is extremely rare. In 1996, Cavanagh reported delayed oral extrusion of synthetic C4–C5 graft (14 mm × 8 mm), made of polymer [16]. In 2001, Sharma reported delayed pharyngeal perforation and oral extrusion of C2–C3 acrylic graft with Kirschner's wire [17]. In 2000, Fujibayashi reported an asymptomatic migration of



**Fig. 4 – Intraoperative photography, demonstrating posterior pharyngeal wall with the wound made by Biocage (arrows).**

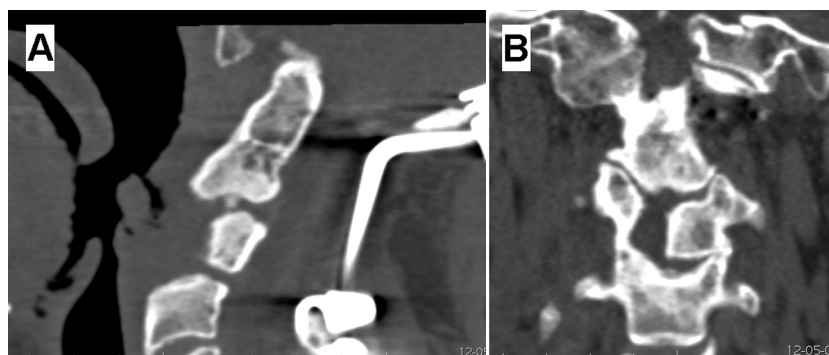

**Fig. 5 – CT of the cervical spine performed few hours after extrusion of Biocage. Sagittal (A) and frontal (B) image reconstructions, demonstrating absence of implant in surgically created space between C2 and C4.**

cervical 25-mm plate with four screws through pharyngeal wall, implants were eliminated through the gastrointestinal tract [18]. We report an oral extrusion of a relatively large cage (17 mm × 17 mm × 8 mm) covered by bioresorbable layer. What is curious in our case is that control CT performed nine months after implantation evidenced properly positioned Biocage. Extrusion took place twenty-seven months after implantation, when integration of Biocage with surrounding bone could be expected; moreover, stability of Biocage was assured by posterior occipitocervical instrumentation. In opinion of some authors, possibility of a delayed migration or an extrusion of bioabsorbable implants is reduced because the devices dissolve [3–6]. As such implants are the developing branch of biomaterials [5], there are few data about complications associated with their use. To our best knowledge, oral extrusion of bioabsorbable cervical implant has not been previously reported.

### Conflict of interest

None declared.

### Acknowledgement and financial support

None declared.

### Ethics

The work described in this article has been carried out in accordance with The Code of Ethics of the World Medical Association (Declaration of Helsinki) for experiments involving humans; Uniform Requirements for manuscripts submitted to Biomedical journals.

### REFERENCES

- [1] Garrett M, Bartolomei J, Sonntag VKH. Anterior approach for cervical spondylotic myelopathy. In: Winn RH, editor. *Youmans neurological surgery*. 6th ed. Philadelphia: Elsevier Saunders; 2011. p. 2876–87.
- [2] Knaub MA, Herkowitz HN. Anterior approach for cervical myelopathy. In: Herkowitz HN, editor. *Rothman-Simeone the spine*. 5th ed. Philadelphia: Saunders Elsevier; 2006. p. 847–63.
- [3] Lippman CR, Hajjar M, Abshire B, Martin G, Engelman LW, et al. Cervical spine fusion with bioabsorbable cages. *Neurosurg Focus* 2004;16: article 4.
- [4] Pflugmacher R, Schleicher P, Gumnior S, Turan FO, Scholz M, Eidott T, et al. Biomechanical comparison of bioabsorbable cervical spine interbody fusion cages. *Spine* 2004;29:1717–22.
- [5] Robbins MM, Vaccaro AR, Madigan L. The use of bioabsorbable implants in spine surgery. *Neurosurg Focus* 2004;16:article 1.
- [6] Vaccaro AR, Robbins MM, Madigan L, Albert TJ, Smith W, Hilibrand AS. Early findings in a pilot study of anterior cervical fusion in which bioabsorbable interbody spacers were used. *Neurosurg Focus* 2004;16: article 7.
- [7] Söderlund CH, Pointillart V, Pedram M, Andrault G, Vital JM. Radiolucent cage for cervical vertebral reconstruction: a prospective study of 17 cases with 2-year minimum follow-up. *Eur Spine J* 2004;13:685–90.
- [8] Cagli S, Isik HS, Zileli M. Cervical screw missing secondary to delayed esophageal fistula: case report. *Turk Neurosurg* 2009;19:437–40.
- [9] Geyer TE, Foy MA. Oral extrusion of a screw after anterior cervical spine plating. *Spine* 2001;26:1814–6.
- [10] Finiels P-J, Hernandez G, Sabatier P, Frerebeau P. Delayed esophageal perforation after cervical osteosynthesis. Case illustration. *J Neurosurg* 2000;92:123.
- [11] Lee JS, Kang D-H, Hwang SH, Han JW. Oral extrusion of screw after anterior cervical interbody fusion. *J Korean Neurosurg Soc* 2008;44:259–61.
- [12] Martinez-Lage JF, Felipe-Murcia M, Martinez-Lage Azorin L. Late prevertebral abscess following anterior cervical plating: the missing screw. *Neurocirurgia* 2007;18: 111–4.
- [13] Pompili A, Canitano S, Caroli F, Caterino M, Crecco M, Raus L. Asymptomatic esophageal perforation caused by late screw migration after anterior cervical plating. *Spine* 2002;27:E499–502.
- [14] Wong DT, Fehlings MG, Massicotte EM. Anterior cervical screw extrusion leading to acute upper airway obstruction. *Spine* 2005;30:E683–6.
- [15] Fountas KN, Kapsalaki EZ, Nikolakakos LG, Smisson HF, Johnston KW, Grigorian AA, et al. Anterior cervical discectomy and fusion associated complications. *Spine* 2007;32:2310–7.
- [16] Cavanagh SP, Tyagi A, Marks P. Extrusion of BOP-B graft orally following anterior cervical discectomy and fusion. *Br J Neurosurg* 1996;10:417–8.
- [17] Sharma RR, Sethu AU, Lad SL, Turel KE, Pawar SJ. Pharyngeal perforation and spontaneous extrusion of the cervical graft with its fixation device: a late complication of C2–C3 fusion via anterior approach. *J Clin Neurosci* 2001;8:464–8.
- [18] Fujibayashi S, Shikata J, Kamiya N, Tanaka C. Missing anterior cervical plate and screws. *Spine* 2000;25:2258–61.