

Radiation protection in cardiac cath labs. Expert review and opinion of the Association of Cardiovascular Interventions, the Working Group on Echocardiography of the Polish Cardiac Society, and the Polish Society of Medical Physics

Krzysztof Milewski^{1,2}, Tomasz Pawłowski³, Joanna Kidoń-Szołtysek^{4,5}, Mariusz Tomaniak⁶, Bartłomiej Góra², Piotr Barus⁶, Andrzej Gackowski⁷, Piotr Szymański^{8,9}, Katarzyna Mizia-Stec¹⁰, Andrzej Lekston¹¹, Michał Hawranek¹¹, Marek Grygier¹², Tomasz Piotrowski^{13,14}, Wojciech Wojakowski¹⁵

¹Academy of Silesia, Faculty of Medicine, Katowice, Poland

²Cardiology and Cardiac Surgery Center in Bielsko-Biala, American Heart of Poland, Bielsko-Biala, Poland

³Department of Cardiology, National Institute of Medicine of the Ministry of Interior and Administration, Warszawa, Poland

⁴Department of Invasive Cardiology and Electrophysiology, Medical University of Silesia, Katowice, Poland

⁵Department of Medical Physics, Leszek Giec Upper-Silesian Medical Center of the Medical University of Silesia, Katowice, Poland

⁶1st Department of Cardiology, Medical University of Warsaw, Warszawa, Poland

⁷Noninvasive Cardiovascular Laboratory, John Paul II Hospital, Kraków, Poland

⁸Department of Noninvasive Cardiovascular Diagnostic, Clinical Cardiology Center, National Institute of Medicine of the Ministry of Interior and Administration, Warszawa, Poland

⁹Center for Postgraduate Medical Education, Warszawa, Poland

¹⁰1st Department of Cardiology, School of Medicine in Katowice, Medical University of Silesia, Katowice, Poland

¹¹3rd Department of Cardiology, Silesian Centre for Heart Disease, Medical University of Silesia, Zabrze, Poland

¹²1st Department of Cardiology, Poznan University of Medical Sciences, Poznań, Poland

¹³Department of Electroradiology, Poznan University of Medical Sciences, Poznań, Poland

¹⁴Department of Medical Physics, Greater Poland Cancer Centre, Poznań, Poland

¹⁵Department of Cardiology and Structural Heart Diseases, Medical University of Silesia, Katowice, Poland

Correspondence to:

Prof. Krzysztof Milewski, MD, PhD,
Cardiology and Cardiac Surgery
Center in Bielsko-Biala,
American Heart of Poland,
phone: +48 33 472 63 00,
e-mail:

krzysztof.milewski@ahop.pl

Copyright by the Author(s), 2024

DOI: 10.33963/v.phj.103632

Received:

November 4, 2024

Accepted:

November 4, 2024

Early publication date:

November 18, 2024

A B S T R A C T

The number and complexity of percutaneous interventions performed by cardiologists, vascular surgeons, and radiologists are constantly growing. These procedures utilize ionizing radiation that, on some occasions, can be significant, causing a serious health hazard for medical team members, including physicians, nurses, technicians, and, more frequently, echocardiographers, anaesthesiologists, and medical physicists. All these groups require special attention, including law regulations, training, protection against radiation that uses modern angiographs and shields, monitoring, and treatment. This multidisciplinary approach may significantly decrease their and patients' health-related burden. This article aims to comprehensively review the basics of ionizing radiation, principles of protection against radiation, organization of radiology catheterization laboratories, formal and legal requirements for the personnel, and discuss medical consequences of X-ray radiation.

Key words: invasive cardiology, invasive radiology, ionizing radiation, occupational hazard, protection against radiation

INTRODUCTION

For decades, the number of percutaneous interventions performed in cardiology, vascular surgery, and radiology has constantly grown. These procedures use ionizing radiation that allows for the visualization of anatomical structures. Unfortunately, radiation exposure can be significant and may cause serious health risks for the entire medical team working close to the radiation source. Many conditions, including cancer, cataracts, neurodegenerative disorders, hypertension, radiation-induced cardiac dysfunction, and others, have been reported among interventional cardiologists [1, 2]. It is also well known that physicians specialized in performing percutaneous interventions have the highest radiation exposure of all professions, significantly exceeding the yearly dose of nuclear power plant workers [3].

These facts indicate that protection against radiation should play a significant role in the everyday work of each medical team member. This article is a comprehensive review that explains the basics of ionizing radiation, principles of protection against radiation, the organization of radiology catheterization laboratories, and formal and legal requirements for personnel; it also discusses the medical consequences of X-ray radiation.

BASICS OF IONIZING RADIATION

Ionizing radiation is generated by bombarding a target (e.g., tungsten) with electrons whose kinetic energy is of the order of keV [4]. X-rays can ionize the medium through which they pass and are harmful to living organisms.

The absorbed dose is the basic quantity used in protection against radiation. According to the definition, it is the energy deposited in the mass element of the medium. The SI unit of absorbed dose is Gray [$1\text{Gy} = \frac{\text{J}}{\text{kg}}$]. Regarding imaging procedures (diagnostic energy range of X-type ionizing radiation), the dose absorbed in a given material equals kinetic energy released per unit mass (kerma) [5]. This means that the kinetic energy imparted to the mass is wholly absorbed in this range.

The effective dose (E) is the sum of equivalent doses (H_T) from external and internal radiation in all organs (tissues), considering appropriate weighting factors [6, 7]. For X-ray energy radiation, an effective dose of 1 Sv produces the same stochastic effects as an absorbed dose of 1 Gy, assuming uniform whole-body irradiation with ionizing radiation with a weighting factor of 1 (e.g., X-rays). Equivalent doses should be considered for all organs/tissues in the human body that are perceived to be sensitive to stochastic effects. E is determined for a reference human. Therefore, an effective dose should be used for comparative purposes (for example, medical procedures and radiological devices) rather than for a specific person [7].

Equivalent dose (H_T) takes into account differences in relative biological effectiveness (RBE) of different types of ionizing radiation (X, gamma, alpha, beta, neutrons).

Siewert is the equivalent and effective dose SI unit [$1\text{Sv} = \frac{\text{J}}{\text{kg}}$].

IONISING RADIATION — DOSE LIMITS

According to the Polish Atomic Law, the dose limit is the value of the ionizing radiation dose, expressed as an effective or equivalent dose. This limit is set for specific groups engaged in controlled professional activities and, except for cases outlined in the Polish Atomic Law, must not be exceeded [8]. The Polish Atomic Law introduces additional concepts of dose constraints (usable dose limit), which should be considered when planning radiological protection for optimization purposes.

Under current regulations, the dose limit for employees occupationally exposed to ionizing radiation is 20 mSv/year, expressed as an effective dose. This dose may be exceeded by the specific conditions specified in the Polish Atomic Law. Poland's workers exposed to ionizing radiation are divided into A and B categories. The first covers workers who may be exposed to an annual effective dose exceeding 6 mSv or an equivalent dose exceeding 15 mSv per year for eye lenses or 150 mSv per year for skin or limbs. Category B includes employees not included in Category A [8]. So far, no dose limits have been established for occupational exposure to the brain [9].

Changes regarding the dose limit values in the Polish Atomic Law (2023) relate primarily to lowering the dose threshold for eye lenses. They were introduced following the recommendations of the International Commission on Radiological Protection (ICRP) in connection with scientific reports suggesting the occurrence of deterministic effects on the eye lens at much lower doses than previously assumed, also because of chronic occupational exposure to ionizing radiation [10]. The annual dose limit expressed as the dose equivalent to the eye lens is 20 mSv. This value (in a given calendar year) may be exceeded up to 50 mSv, provided that over the next 5 years (including the year the dose was exceeded), it may not exceed 100 mSv [8]. The ICRP 139 report defines the value of the average dose per eye lens for the operator of an X-ray treatment unit in the range of 40 to 60 μSv /procedure (DSA, angioplasty, embolization). Considering the specificity of the staff's work in the environment of the X-ray treatment unit, the eye lens closest to the source of ionizing radiation is the most exposed. In the case of improper use or lack of anti-radiation shields and with many procedures performed, the 20 mSv/year limit can be easily exceeded. Studies conducted in recent years have shown that the value of the annual equivalent dose for the lens can reach even 50–100 mSv [10].

The effective dose for cardiology/interventional radiology department employees depends on the specifics of the work (operator, nurse, anaesthesiologist, echocardiographer) and, thus, the location related to the radiation source and the type of anti-radiation shields used. According to the ICRP 139 report, the typical value of the effective dose

received during the year by professionally active operators working in interventional radiology is up to 2–4 mSv [10]. Measurements among interventional cardiologists showed that the effective dose received during a single medical procedure ranges from 0.2 μ Sv to over 100 μ Sv, with an average value between 8 and 10 μ Sv [11]. Considering the procedures in which the effective dose is 10 μ Sv/procedure, the annual value of the effective dose may even reach 10 mSv [10] for active interventional cardiologists performing about 500 procedures a year and even 300 mSv during thirty years of professional work [11]. Studies conducted among 14 interventional cardiologists from nine hospitals in Norway showed an annual effective dose in the range of 1–11 mSv, with an average value of 5 mSv [12]. The measurement methodology was based on two dosimeters placed under and over the individual anti-radiation shield. On the other hand, measurements made in the hospital in Glasgow among interventional cardiologists, using one dosimeter placed under a personal cover, showed the maximum annual effective dose of 1.2 mSv [10].

The pioneering work of Crowhurst et al. [13] on the X-ray exposure of echocardiographers monitoring percutaneous procedures showed that this exposure is at least as high as that of the first operator. The observation mainly concerned transcatheter aortic valve replacement interventions, in which the echocardiographer was positioned at the head of the patient, toward the patient's left side, and stood obliquely, predominantly with their back to the X-ray source. Procedures using predominantly right anterior oblique (RAO) and steep RAO projections were associated with higher exposition to radiation than posteroanterior (PA), left anterior oblique (LAO), and steep LAO. In conclusion, it should be underscored that the dose is lower anytime a person faces the X-ray lamp and higher while a person stands next to it.

MEDICAL CONSEQUENCES OF X-RAY RADIATION FOR PERSONNEL

Over the last decades, there has been a rapid increase in the application of radioactive substances and ionizing radiation in several disciplines, including interventional cardiology [14, 15]. Due to the vast development of radiology techniques, the number of people affected by long-term radiation exposure worldwide is large. It is estimated that practicing interventional cardiologists' exposure equals approximately 250 chest X-rays each year. For a patient, coronary angiogram carries a radiation exposure of around 350 chest X-rays (range 100–800), whereas percutaneous coronary intervention (PCI) corresponds to about 750 chest X-rays (range 350–2650) [16]. Understanding the potential radiation-related health hazards among the catheterization laboratory staff is crucial to improving cutaneous radiation syndrome prevention and early detection.

A study based on the National Dose Registry of Canada extracted data about a cohort of 67 562 medical workers (23 580 males and 43 982 females) regarding mortality and

cancer incidence. The cohort worked with ionizing radiation in various fields of medicine, not specifically in invasive cardiology, over 36 years (1951–1987). The mortality caused by cancer and non-cancer causes was below expected as compared to the general Canadian population. However, thyroid cancer incidence was significantly elevated both among males and females [17]. A decreasing trend in radiation doses obtained from dosimeters in the later years was observed, which can be reasonably explained by better and safer medical equipment and stricter radiological protection guidelines [18].

Another disease associated with ionizing radiation in medical personnel is eye cataract [19]. One study examined the prevalence of lens opacities in interventional cardiologists and nurses. Among interventional cardiologists, 52% were diagnosed with radiation-associated posterior lens opacities, and in 45% of nurses, the same disease was found. On the other hand, lens opacities were present only in 9% of the control group. The relative risk for interventional cardiologists was 5.7% and 5.0% for nurses [20]. A study by Chodick et al. [21] presented the results of a prospective study involving a cohort of 35 705 US radiologic technologists aged 24–44 years who did not suffer from eye cataracts at baseline. The study group mainly consisted of females (82.6%), and 66% of the radiologic technologists started working aged 20 or younger. The follow-up was nearly 20 years long and involved two questionnaires. During this period, 2382 cataracts (591 before 50 years of age) and 647 cataract extractions were reported (183 before 50 years of age) — the risk of developing a cataract increased by 15 percent per year. Moreover, increased cataract risk and extraction were observed with a growing number of personal diagnostic X-rays. Several comorbidities at baseline were associated with an increased risk of an eye cataract, e.g., smoking tobacco (≥ 5 pack-years), BMI ≥ 25 kg/m², diabetes mellitus, hypertension, hypercholesterolemia, and arthritis [21].

An analysis by Khafaji et al. [22] showed that in pediatric interventional cardiologists, a significant difference was found between the left and the right eye measurements ($P = 0.034$), with higher doses administered to the left eye. Interestingly, the authors also measured thyroid and did not find any differences between the right and left thyroid doses ($P = 0.281$) [22].

Several studies have touched on the matter of breast cancer and skin cancer among medical staff working with ionizing radiation, mainly radiologic technicians [23–25]. A study by Doody et al. evaluated the incidence of breast cancer between 1983 and 1998 among 56 436 female radiologic technicians who were certified from 1925 to 1980. Breast cancer risk was significantly increased among staff experiencing low doses of radiation over several years, presumably resulting in a high cumulative exposure. With the introduction of new, improved technology and protection, the risk of breast cancer decreased in relation to the total years worked before 1940, but not after [25]. Yoshinaga and all emphasize that there is no clear evidence

of an increased risk of cancer in medical workers currently exposed to ionizing radiation. However, one should bear in mind the relatively short period of observation of these workers and the increase in the use of radiation in medicine. Hence, further observation of their health is critical.

Ionizing radiation can also cause DNA and chromosome damage among medical personnel [26–28]. A study by Gaetani et al. [29] evaluated the influence of low doses of ionizing radiation on DNA damage in the cells of medical workers. The study population was assigned to two groups depending on the exposure dose, with 6 mSv/year being the dividing point. Both groups were compared to a control group of healthy individuals who had never been occupationally exposed. The DNA of lymphocytes was analyzed in terms of single-strand breaks, oxidized pyrimidine, and purine bases, all of which are markers for DNA damage. DNA repair was measured concerning repair activity, amount of repaired DNA and half-time to repair DNA damage. In both groups subjected to chronic low-dose ionizing radiation, the DNA repair activity was increased; however, only the group with high exposure accumulated DNA damage in lymphocytes. Moreover, a significant accumulation of DNA damage and reduced repair activity of one mechanism were found among subjects who had a family history of cancer. The authors concluded that low-dose ionizing radiation in occupational settings may be mutagenic, thus leading to cancer [29]. Nonetheless, extensive prospective cohort studies must be performed to confirm this thesis. Another study found increased chromosomal aberrations and sister chromatid exchanges in hospital radiation workers, indicating a cumulative effect of low-level, chronic ionizing radiation exposure [30]. The cytokinesis-block micronucleus is a reliable marker of radiation-induced chromosome damage [31]. A study on Tunisian hospital workers assessed the lymphocytes of 67 workers exposed to low levels of ionizing radiation and compared the results to a control group of 43 people. A significant increase of cytokinesis-block micronucleus among medical workers was found. Multivariate regression analysis showed that only the exposure time to ionizing radiation significantly impacted the level of cytokinesis-block micronucleus [32]. However, the direct and long-term impact of such DNA and chromosome changes on health is unknown.

FORMAL AND LEGAL REQUIREMENTS FOR THE CARDIOLOGY CATHETERISATION LABORATORY PERSONNEL

Staff employed in the cardiology catheterization laboratories should meet certain conditions both in terms of qualifications and health requirements. These conditions are related to direct exposure to ionizing radiation and the need to minimize patient and medical personnel's health risks. The current Polish regulations [33] define the minimum conditions for providing health services in X-ray diagnostics and interventional radiology. Based on this legal act, the interventional cardiology (and radiology)

laboratory should have an X-ray system with appropriate software and equipment to perform vascular procedures, including radiation shielding.

The cardiac catheterization laboratory staff must include at least one physician specialized in the field of medicine, corresponding to the radiological procedures performed, with current certification from the accredited body. In the case of cardiologists, this condition is met by completing a specialization program and by obtaining a certificate of an independent diagnostician and independent operator issued by the Association of Cardiovascular Interventions of the Polish Cardiac Society (AISN PTK, *Asocjacja Interwencji Sercowo-Naczyniowych Polskiego Towarzystwa Kardiologicznego*). The importance of these documents was confirmed by the Notice of the Minister of Health on Radiological Reference Procedures of 2015 [34].

In addition, a radiology technician and a nurse (if administration of a contrast medium is required) must be employed in the invasive cardiology laboratory. The regulations indicate that the employment of a nurse is necessary when other personnel do not have the appropriate qualifications to administer the contrast agent. In the case of an invasive cardiology laboratory, this condition is met by a specialist cardiology physician. However, it should be emphasized that nurses in invasive cardiology laboratories perform other tasks related to the instrumentation of procedures and assistance for the instrumenting nurse. Unfortunately, this is not reflected in the legal provisions developed by the AISN PTK and should be defined as part of the organizational standard for invasive cardiology laboratories.

A specialist in medical physics or a person authorized by the head of the healthcare unit to perform tasks in X-ray diagnostics or interventional radiology referred to in Art. 33h sections 9 and 10 of the Polish Atomic Law (a medical physicist in the field of X-ray diagnostics and interventional radiology) supports the personnel in the catheterization laboratory [8]. These qualifications are required to ensure the optimization of radiological protection for patients and other exposed people, define quality criteria for radiological devices, prepare technical specifications of radiological devices and auxiliary devices, and select devices needed to conduct measurements in the protective field against ionizing radiation. In addition, that specialist must analyze any incidents of unintentional or accidental exposure. At this point, it should be noted that one medical physicist should be employed in a healthcare unit for every 20 000 radiological procedures carried out annually.

A separate problem concerning the personnel of the invasive cardiology laboratory is the health protection of the employees employed in a catheterization laboratory. The requirements regulating that matter are specified in several articles of the Polish Atomic Law, in particular in Art. 14 (pregnant or breastfeeding employees), Art. 17 (employee categories), and Art. 30 (medical supervision of employees, medical documentation) [8].

In addition, it should be emphasized that the Act introduces two categories of employees exposed to ionizing radiation: A and B, as mentioned earlier. Category A employees should have periodic examinations yearly. This category may apply to operators of surgical X-ray units due to the dose per lens exceeding 15 mSv (Polish Atomic Law, Art. 17.1.1.b). A medical certificate confirming the employee's ability to do his/her job should be kept in records for inspection by authorized inspection bodies. This rule applies to employees working under an employment contract, civil law, or other contracts.

Another mechanism for controlling the degree of exposure to ionizing radiation is the introduction of a dosimetry passport, which collects data on employees' exposure to ionizing radiation, into the legal system. This is particularly important in the case of external employees providing services in many healthcare units. The dosimetry passport allows for individual personnel exposure monitoring and quicker capture of situations that force the employee to be referred for periodic examinations. The dosimetry passport is issued by the President of the Atomic Energy Agency upon a written request. Detailed regulations are contained in the Regulation of the Council of Ministers of November 30, 2020 [35]. It is a formal requirement for the staff of the invasive cardiology laboratory to do training on protection against radiation confirmed by a certificate — this has been discussed in Chapter 9 [8].

The invasive cardiology laboratory, as well as other units that use ionizing radiation, should cooperate with the inspector overseeing protection against radiation, who is responsible for ensuring compliance with radiological protection requirements and may conduct an operational assessment of the level of exposure to ionizing radiation of individual employees on an ongoing basis, as well as participate in commissioning and operation of angiographic devices for interventional radiology. The scope of powers of the radiological protection inspector is defined in the Polish Atomic Law (Art. 7) and the Regulation of the Minister of Health [36].

RADIOLOGICAL PROTECTION OF PATIENTS (INCLUDING SPECIAL POPULATIONS — PREGNANT WOMEN AND CHILDREN)

Per the Polish Atomic Law Act, radiological protection of the patient is a set of activities and restrictions aimed at minimizing the patient's exposure to ionizing radiation, which will not excessively hinder or prevent obtaining the desired and justified diagnostic information or therapeutic effects. Legal requirements regarding the use of ionizing radiation for medical purposes and non-medical imaging are included in Chapter 3a of the Polish Atomic Law Act [8].

Cutaneous radiation injury

Cardiology and interventional radiology procedures (especially therapeutic interventions) often generate doses of ionizing radiation to the patient's skin that are compa-

rable to or higher than the daily fractional dose received in radiation therapy for cancer treatment (2 Gy).

Skin damage is one of the primary deterministic effects caused by ionizing radiation. They take the form of cutaneous radiation injury (CRI), which covers the skin, subcutaneous fat layer, and muscle [37]. Scientific reports on skin damage and epilation under the influence of X-ray radiation from the range used in radiological diagnostics are mainly described in the case of computed tomography scans (brain perfusion) and PCIs [38]. The timing and severity of the individual effects of CRI depend on the dose and other factors (Figure 1). For a single fraction of radiation, the threshold for the appearance of a transient form of erythema is about 2 Gy, a definite form of erythema is about 6 Gy, and about 3 Gy for transient epilation [39]. Most severe skin damage occurs 4 to 8 weeks after exposure (Table 1).

It should be noted that these dose thresholds are approximate values, which are affected by different individual sensitivity to ionizing radiation and other factors. The most common predictive factors include obesity and irradiation of the part of the skin previously exposed to ionizing radiation [9, 38].

If it is necessary to repeat the procedure using ionizing radiation, it is important to maintain an appropriate time interval if the patient's condition allows it. This time is related to repairing sublethal damage and repopulation, i.e., proliferation (multiplication) of cells that survived irradiation. The first process usually ends within 24 hours, and the second lasts several months [37]. Repopulation begins much later (about two weeks after irradiation) and lasts longer if the absorbed dose is higher because the number of surviving cells decreases with increasing the dose. Post-radiation skin lesions are similar in size to the beam field on the patient's skin, where the threshold dose value has been deposited (single beam/overlapping fields of different beams — so-called hot spots) [9]. In addition to the deterministic effects discussed above, even low-dose irradiation can lead to stochastic impacts (skin cancers) with a latency period of more than 15 years [38].

In diagnostic examinations that use ionizing radiation, patients' effective doses should be limited to the lowest possible level. This level should ensure obtaining an examination result of the expected diagnostic quality. Optimization of the patient's radiological protection is also achieved by reducing the number of unnecessary repeat examinations. In addition, in interventional radiology/cardiology, necessary steps should be taken to prevent radiation damage to the skin and underlying tissues as a result of long-term exposure, particularly with a high-dose X-ray beam (Polish Atomic Law, Art. 33d p. 2, 3) [8].

In Polish legal recommendations [40], there were two response thresholds for the skin dose (i.e., the dose to the patient's skin, including scattered radiation): 1 Gy and 3 Gy. However, since the skin dose is difficult to calculate, and programs capable of performing such calculations are not routinely used in clinical practice, the two recently

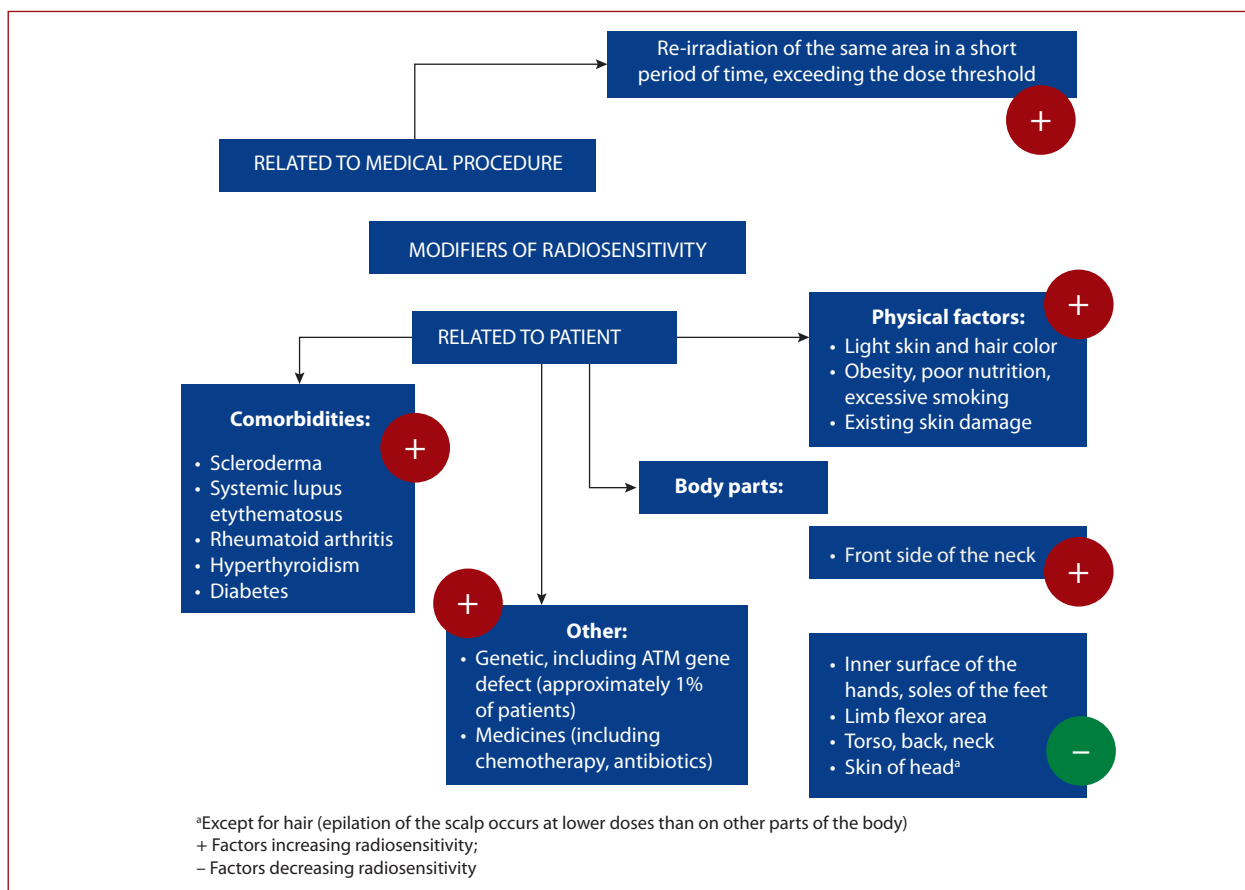


Figure 1. Factors influencing variable radiosensitivity [9]

Table 1. The course of radiation skin syndrome in the case of single-dose irradiation [9]

Effect	Radiation dose, Gy ^a	Time of occurrence	Time of maximum presentation
Transient erythematous phase	2	Hours	~ 24 h
Transient epilation	3	~ 3 weeks	-
Main erythematous phase	6	~ 10 days	~ 2 weeks
Permanent epilation	7	~ 3 weeks	-
Skin atrophy (1 phase)	10	>52 weeks	-
Telangiectasias	>12	>52 weeks	-
Dry desquamation	14	~ 4 weeks	-
Late erythematous phase	15	8–10 weeks	-
Moist desquamation	18	~ 4 weeks	-
Dermal atrophy/necrosis	18	>10 weeks	-
Secondary ulceration	20–24	>6 weeks	-

^aSingle exposure, dose to the patient’s skin including scattered radiation, ~ about

published regulations include new dose thresholds: 1.7 Gy (or 170 Gy·cm²) and 5 Gy (or 500 Gy·cm²) [41, 42]. These thresholds refer to the total value of the kerma at the reference point ($K_{air,ref}$) or the DAP parameter (total dose area product — the product of the dose and the X-ray field area), i.e., the parameters included in the dosimetry report generated after the end of the examination/procedure. During exposure, these parameters are also visible on the X-ray monitor of the X-ray unit. When the threshold of 1.7 Gy (or 170 Gy·cm²) is exceeded, the patient’s medical documentation should record information about the dose. The referring physician should provide that information

if the procedure requires repeating (referring physician — a physician, dentist, or other person authorized to refer people for medical radiological procedures [Polish Atomic Law Act]) [41].

In the second case (5 Gy or 500 Gy·cm²), the patient should undergo control examinations in the medical unit performing the procedure at least once a week within 21 days following the exposure [42]. In addition, exceeding the threshold of 5 Gy or 500 Gy·cm² should be classified as a category II event (unintentional exposures and accidental exposures) if, within 21 days of the interventional procedure, skin damage of at least second-degree occurs due to

Table 2. Dose notification levels according to National Council on Radiation Protection and Measurements No. 168 [43]

Dosimetric parameters	First notification level	Second notification (increments)	Substantial radiation dose limits (SRDL)
PSD, Gy	2	0.5	3
$K_{air,ref}$ Gy	3	1	5
DAP, Gy·cm ²	300	100	500 ^a
FT, min	30	15	60

^aFor field at the patient's skin equal 100 cm², for other fields the DAP needs to be adjusted proportionally (e.g. for 25 cm² the SRDL would be 125 Gy·cm²)

Abbreviations: DAP, dose area product; FT, fluoroscopy time; $K_{air,ref}$, air kerma at X-ray unit reference point; PSD, peak skin dose

radiation [41]. If the dose exceeds 5 Gy or 500 Gy·cm², the patient must undergo a follow-up examination, including at least his/her skin inspection. Category II events in the field of interventional radiology also include (in the absence of clinical justification) four times the value of the diagnostic reference level and, in the case of procedures carried out for diagnostic purposes — exceeding 2.5 Gy of the total value of kerma in the air at the reference point or 250 Gy·cm² of the total DAP.

Unjustified repetition of an interventional procedure leading to a cumulative dose exceeding the above levels is classified as a category I event, including performing a procedure that results in an unexpected deterministic effect, performing the procedure on a wrongly identified person, and procedures in the wrong anatomical area. A protocol is drawn up from the events, which should be submitted to the appropriate national or voivodeship consultant in the relevant medical field related to the use of ionizing radiation and to the National Center for Radiological Protection in Healthcare.

The National Council on Radiation Protection and Measurements, in report no. 168 from 2010, recommends additionally introducing a threshold for peak skin dose and fluoroscopy time (Table 2) [38, 43].

It is essential to note that the value of the DAP parameter refers to a specific field dimension. This means that this level should be lower in procedures such as cardiology or neurology. The fluoroscopy time is not a good indicator. It should be used in conjunction with other levels, as it only informs about fluoroscopy duration without such important information as X-ray dose rate or pulsed fluoroscopy parameters. Fluoroscopy time is related to the dose rate of ionizing radiation. Therefore, its monitoring is justified (a higher dose value in a shorter time vs. a lower dose value in a longer time).

Reference levels

We do not use ionizing radiation dose limits for patients. Instead, diagnostic reference levels (DRL) are utilized to assess and optimize patient exposure. According to the Polish Atomic Law, DRL in interventional radiology is the level of ionizing radiation dose in typical diagnostic examinations/interventional procedures performed on patients with a standard body structure concerning broadly defined equipment categories.

Table 3. Diagnostic reference levels for adults in Poland; based on [50]

Type of procedure	Dose area product, Gy·cm ²	Exposure time, min
Phlebography of the lower limbs and pelvis	9	–
Arteriography of the lower limbs and pelvis	85	–
Coronary angiography	60	–
Percutaneous transluminal angioplasty	100	18
Percutaneous coronary intervention	120	20

Table 4. The proposed diagnostic reference levels for interventional cardiology for adults; based on [37]

Type of the procedure	KAP, Gy·cm ²
Coronary angiography	35
Percutaneous coronary intervention	85
Transcatheter aortic valve implantation	130
Electrophysiological procedures	12
Pacemaker implantation	Single-chamber — 2.5 Dual-chamber — 3.5 Resynchronization pacemaker — 18

Table 3 shows established and proposed DRLs for interventional radiology procedures—notably, there are few procedures for which DRLs have been published in Poland. So far, no diagnostic reference levels have been established in Poland for pediatric interventional procedures. In the literature, there are publications about the values of diagnostic reference levels for procedures other than those listed in Table 3 (see Table 4) [44–49] and procedures carried out in Polish hospitals.

Factors affecting X-ray dose

Factors influencing the dose can be divided into those dependent on the X-ray machine, operator, or patient.

Medical procedures performed under the supervision of fluoroscopy are characterized by the most variable dose values for a single procedure [11]. Thus, in interventional cardiology, both patients and staff can receive high doses of ionizing radiation. The primary beam of ionizing radiation generated by the X-ray tube is the main source of radiation reaching the patient. Proper patient placement in the X-ray tube-image detector system affects the operation of the

automatic exposure and image quality control system. This system is sensitive to many factors depending primarily on the radiological thickness (the patient and all elements in the field of view of the radiation beam, including the patient's body, table, mattress [silicone mattresses increase the exposure parameters], or collimator shutters [blinds] if they are in the active area of the image detector [applies to flat digital/panel detectors]) and the geometry of the X-ray tube, the patient, and the image detector system [9]. Placing the patient too low will bring the patient too close to the source of ionizing radiation and negatively affect the dose he/she receives. However, placing them too high will also cause the image detector to move away from the X-ray tube. Thus, it will be necessary to increase its efficiency so that the determined dose value at the level of the image detector is achieved. By good clinical practice, the image detector should be placed as close as possible to the patient's body, thus eliminating unnecessary geometric magnification that generates a higher dose. This solution makes the detector absorb part of the scattered radiation generated by the patient, which reduces the exposure of the personnel standing nearby [11]. Radiation scattered on the surface of the image detector may also cause image quality degradation [9].

The parameters of the primary source, which directly affect the dose received by the patient, include accelerating voltage (kV)/peak voltage (kVp), half value layer (HVL in mm Al), beam-filtration (in mm Al) to absorb low energy photons, detector field of view size, magnification, brightness optimization system (sensor, optimization algorithm), LIH option (last image hold function), fluoroscopy duration, image acquisition time and clinical protocol parameters related to these times, i.e., current (mA), continuous fluoroscopy mode/pulse (frames per second [fps]), pulse length (ms), dose per pulse (typically in nGy/pulse), pulse power (pulse/s), additional filtration, and the size of the primary beam field (collimation) [9].

It is essential to control proper operation of the X-ray device, its calibration, and quality to maintain accuracy. It should be noted that, per the Polish Atomic Law, X-ray equipment may not be used if quality control tests have not been carried out with the appropriate frequency and if the results of these tests are outside the tolerance range.

Pregnancy

Particular protection concerning medical exposure applies to, among others, women of childbearing age, pregnant women, and patients under 16. Performing an examination or procedure using ionizing radiation in a pregnant woman is possible only if the alternative examinations, procedures, or postpartum treatments do not provide important clinical information or do not bring the desired therapeutic effect [8].

In interventional radiology, the attending physician must ensure the exposed woman is not pregnant (the attending physician — a doctor, dentist, or other person

authorized to assume responsibility for subjecting a patient to medical exposure [Atomic Law Act]). In a situation where a woman is pregnant (or when pregnancy cannot be ruled out), particular attention should be paid to indication for the examination/procedure in the field of interventional radiology, medical indications, and optimization of exposure of the pregnant woman and the unborn child, with particular emphasis on the abdominal or pelvic area. In the case of exposure in this area, the healthcare unit is obliged to assess the dose of ionizing radiation for the unborn child.

According to the Minister of Health's regulation on the special protection of specific categories of people in connection with medical exposure in diagnostic examinations, procedures, and treatment, the woman should be informed about the results of this assessment immediately after the examination or procedure [51].

Optimization of radiological protection of pregnant women should be carried out with the participation of a specialist in the field of medical physics or a medical physicist in the field of X-ray diagnostics and interventional radiology, referred to in the Atomic Law. Performing a diagnostic examination or surgery in the abdominal cavity of a pregnant woman, if the pregnancy status has been established after the procedure, and the dose to the embryo or fetus exceeds 20 mSv, is classified as category III of the events (referred to above) unless the intervention was directly related to saving the life of a pregnant woman.

RADIATION PROTECTION SYSTEMS

Anti-radiation shields

The set of anti-radiation shields used in the cardiology/interventional radiology laboratory includes personal shields (e.g., aprons, suits, thyroid shields — item 4 of the photo in [Figure 2](#), as well as glasses and visors), collective protective equipment (screens, ceiling shields, curtains — items 3, 2, 1 of the photo in [Figure 2](#)), shields for the patient and fixed shields (according to the design of the fixed shields, they constitute barriers for protective zones in the laboratory). Personal shields can be individual and collective shields. Personal face shields should fit snugly to reduce leakage.

The radiation-absorbing material consists mainly of lead (collective protective equipment, personal shields, patient shields, and fixed shields). However, individual shields are increasingly made of other material that reduces their weight. It involves bismuth or, increasingly more often, a combination of bismuth, antimony, and tin. The parameter describing the degree of protection is the absorption expressed in the equivalent absorption of a thickness of the lead sheet, with the following being most often used: 0.25 mm, 0.35 mm, 0.50 mm Pb or Pb equivalent (eq.). The transmission of ionizing radiation through the shield is a variable value and depends on the radiological thickness of the shield and the parameters of the X-ray beam [9]. Exemplary literature data indicate that for the voltage range



Figure 2. A set of anti-radiation shields in the cath-lab (own figure), 1 — curtain, 2 — ceiling cover, 3 — screen, 4 — personal shields [9]

of 70–100 kVp, the transmission is typically 0.5%–5.0% [52], where 0.5 mm eq. Pb absorbs 95% of radiation at 70 kVp and 85% at 100 kVp [11].

Shields of lightweight or lead-free materials do not have the same X-ray transmission values as lead ones. Light materials are more effective (excellent radiation absorption), in the energy range of 40–88 keV compared to lead. Therefore, they are recommended for potential acceleration voltages reaching the range of 70–80 kVp [53]. The combination of light elements (antimony with $Z = 52$ or tin with $Z = 50$) with heavier elements (bismuth with $Z = 83$ or lead with $Z = 82$, absorbing radiation more effectively >88 keV) allows minimizing the weight of the shield while maximizing radiation absorption in significant X-ray energy bands used in diagnostics. This shielding material consists of two layers: the antimony closer to the X-ray source and the heavier element closer to the body. The layer of the heavier element, apart from absorbing photons with higher energies, also absorbs the secondary fluorescent radiation generated in the first layer [9]. What is important, secondary scatter radiation from the patient is typically lower in energy, around 4–55 keV.

The basic factor protecting the operator's head and neck is the use of a ceiling shield (usually 0.5–1.0 mm Pb), reducing the dose received in these areas from 2 to 10 times (this value is variable depending on the correct use of the shield) [53], and the eye dose by a factor of 19 [11]. Adding a flexible shield curtain attached to the lower border of the rigid acrylic shield allows the shield to approximate the patient's body better and markedly improves shielding effectiveness, including protecting the operator's hand [54].

In clinical trials with interventional procedures and phantom simulations, the dose reduction factor (DRF) of

ceiling suspensions (including lead panes) is 0.7–19. Higher DRF values have been achieved in studies where ceiling cups have been precisely positioned [53].

A properly placed ceiling shield should be directly above the irradiated area of the patient's body, and the operator should look through it at the irradiated area [9]. In interventional procedures in which a variable angle of the primary beam is used (variable angulation of the C-arm), movement of the operating table and correct placement of the ceiling shield requires relocation, as the X-ray gantry and table are moved, which can be quite burdensome, reducing the effectiveness of the shielding. The protection of the head area of the personnel working in the environment of the X-ray treatment unit is also provided by face shields and protective glasses. The largest part of the scattered radiation reaches from below to the upper parts of the operator's body and assisting personnel [9].

For most of the examination/procedure, the operator looks at the monitors presenting the fluoroscopic acquisition image. Therefore, his eyes are not directly directed at the source of scattered radiation. In this situation, the radiation can reach the eyes through the gap between the glasses and the face, generating the largest share of scattered radiation reaching the eyes. Therefore, the correct fit and reinforcement of the frames and sides with protective material is essential. Head protection covers also include protective caps, whose usefulness is intensely discussed and undermined in the literature because ionizing radiation reaches the upper parts of the staff's body almost entirely from the patient's side (scattered radiation), i.e., from below [9]. The effectiveness of visors, protective glasses, or the lack of justification for the use of protective caps in clinical conditions is discussed in the literature [55].

Personal protective equipment also includes protective gloves. However, their use requires increased attention. Manipulation with protected hands in the area of the primary beam of ionizing radiation may increase the radiation emitted by the X-ray units, increasing exposure to ionizing radiation and thus reducing the effectiveness of protective gloves [56]. These gloves (and other high-density items) should, therefore, be kept out of the active area of the image detector so as not to affect the operation of the automatic brightness control (ABC) system [9]. The lower part of the staff's body is covered by curtains attached to the table. Security measures with a thickness of 0.5 mm Pb are routinely used. These curtains reduce the dose received by the legs by a factor of 10 to 20; in practice, however, this value is between 2 and 7 [54, 57].

As can be seen from the above considerations, the selection of appropriate protective measures requires considering the working conditions of the personnel. The following factors should be considered: workplace — distance from the radiation source (first operator, second operator, imager, nurse, support team, radiology technician), location in relation to the source (orientation of the shielded surface), presence and effectiveness of collective protective equipment at the workplace, time of exposure and the settings of the X-ray system (so-called low-dose, high-dose). The selection of a personal cover (apron, suit) always involves a process of optimizing workplace ergonomics (protecting properties versus the weight of the cover). Personal shields must be airtight to do their job. Using them properly and checking their technical condition (visual and X-ray inspection) is crucial [9].

Another approach to reducing radiation dose is using additional shields, plates, or different types of protective surgical drapes. For example, a special board can be placed under the patient's arm, but its effectiveness in reducing radiation is doubtful. One such solution is the Rad Board® patient arm plate. Although the manufacturer claimed that it reduced the radiation dose to 44% and 25% at the waist and neck level, these optimistic observations were not confirmed by subsequent analysis, which brought the opposite results, saying that the operator was more exposed to radiation. This could have been related to the inability to mount the vertical shield used in the control group [58].

Another way to protect the operator involves shields placed below the level of the table where the radiation from the X-ray tube is emitted. In the EXTRA-RAD study, using shields under the table resulted in lower exposure to the radiation dose at the pelvis and chest level of the operator [59]. Another study showed that installing protective curtains leads to a reduction of radiation dose by as much as 64% [60].

Disposable surgical drapes, which absorb ionizing radiation due to tin, antimony, bismuth, or barium content, work similarly. According to the available data, using such drapes reduces the dose delivered to the eye, thyroid,

and hands 12-fold, 25-fold, and 29-fold, respectively [61]. Despite reducing the amount of radiation reaching the operator, the presented solution is associated with doubling the radiation dose received by the patient during the procedure [62].

A similar solution involves sterile, disposable, lead-free RadPad™ drapes (Worldwide Innovations & Technologies, KS, US). They are placed directly on the patient and act by absorbing the scattered radiation coming from the patient and creating a "shadow zone," in which the operator can perform the procedure. Studies have shown that the use of RadPad™ drapes can reduce radiation by 44%–59%, depending on the study [63–66]. In these studies, however, the dose reduction is measured at the chest or neck level; the reduction below the operator's waist is negligible, and the head dose is only modestly reduced.

ADDITIONAL PROTECTIVE SOLUTIONS

Protective clothing is heavy and, combined with the operator's unergonomic posture, may result in back pain and, in the long term, lead to posture defects affecting everyday functioning [67, 68]. The manufacturer of the Zero Gravity® system devised a solution to this problem, aiming to increase protection against radiation while relieving the doctor. This solution uses unique weighted levers to which protective clothing is attached. Such a system reduces operator fatigue and ailments in the osteoarticular system while not limiting freedom of movement [69]. Another solution that gives greater freedom of movement and reduces ergonomic posture risk for the operator is an Exoskeleton-Based Radiation Protection System (StemRad MD). The anti-radiation effectiveness of this solution was confirmed in research conducted by Katsarou et al. [70]. According to the authors, the effects of the StemRad MD exoskeleton-based system are particularly impactful for the brain, eye lens, and head areas.

Free-standing protective cabins, made of materials that absorb ionizing radiation, are also available on the market. Their main advantage is a significant reduction in the dose to which the personnel are exposed. This is possible due to using more radiation-retaining materials compared to protective clothing. Manufacturers of such devices offer various models specific for electrophysiological procedures or interventional cardiology procedures [71]. Doubts are primarily raised by the functionality of this solution, especially during long or complicated procedures. Recently reported on the Cathpax® AIR cabin resulted in a 78% reduction in radiation exposure without affecting the quality of procedures, both in complex PCI and during structural procedures.

The Radiation Shielding System (Radiation Medical Ltd., Tel Aviv, Israel) protects against radiation by using an additional casing, like a tunnel, within the C-arm between the tube and the image intensifier. This reduces the space through which radiation can pass. The outer protective

shell is triggered by the operator using a special button. This system reduces exposure to ionizing radiation by up to 97% [58, 63–66, 72].

Another way of protection is the EggNest- XR™ System (Egg Medical, Arden Hills, MN, US), which aims to protect the entire cath-lab medical team. It is a carbon fiber-based platform with flexible and adjustable modular shielding components. Studies have confirmed its effectiveness in reducing incoming radiation by 91% [63–66].

Finally, when considering protective solutions, one must consider all possible steps to reduce the need for invasive angiography, including proper indications for interventional procedures. Dębski et al. [73] proposed an interesting approach to this topic. The authors showed that vessels with <50% diameter stenosis on quantitative computed tomography and hemodynamically insignificant CTA-derived FFR results might be omitted during coronary angiography. Such an approach would result in substantial reductions in contrast media volume used and patients' exposure to radiation during ICA, while not leading to misdiagnoses.

Robotics based solutions

Robots performing procedures within the coronary arteries are currently a dynamically developing branch of invasive cardiology. The latest generations of these devices enable interventions even in complex lesions, such as interventions within the left main coronary artery. They are characterized by a significant reduction in exposure to ionizing radiation [74–76].

Compared to the previously mentioned solutions, robots make it possible to move the operator away from the radiation source, and the additional barrier reduces the amount of radiation even more effectively. Such products include the Sensei® X robotic system (Hansen Medical, CA, US) designed for cardiology or electrophysiology procedures. Another robot used is the CorPath GRX (Corindus Inc, Waltham, MA, US). Assisted by the CorPath robot, the operators remain in stations additionally protected against radiation, from where they control the entire procedure. The CorPath system was approved by the Food and Drug Administration for PCI in 2012. Unfortunately, the device was recently withdrawn from the market. The only available angioplasty robot is now an R-one device from Robocath company [77, 78].

However, despite progress, robots performing coronary interventions still need to be evaluated in large randomized clinical trials that will confirm the reduction of radiation exposure with a satisfactory angiographic and clinical effect of the intervention [79].

THE ROLE OF OPERATOR AND PERSONNEL TRAINING IN REDUCING RADIATION DOSES

The safe use of ionizing radiation for medical purposes is defined in Chapter 3a of the Polish Atomic Law [8], which also imposes additional obligations on persons using the

sources of ionizing radiation (mentioned earlier) in the treatment process. To fulfill this obligation, individuals performing diagnostic tests, procedures, or treatments involving ionizing radiation and those supervising their performance are required to obtain a minimum of 20 training points within the next 5 years. In addition, the issues of radiological protection of the patient are regulated by European Union documents, particularly the 2013 Euratom Directive [80], which was incorporated into Polish legislation by the Atomic Law and the Regulation of the Minister of Health from March 6, 2020 [81].

These documents define the forms and topics of training for all employees who come into contact with ionizing radiation and define the examination rules, allowing these employees to obtain certificates to work with it. The certificate is issued for five years, after which the training must be repeated. From the point of view of the cath lab, the obligation to undergo training applies to physicians performing interventional radiology procedures (including cardiological procedures) and radiology technicians. Notably, the regulation does not include nurses (nurses have no influence on the patient dose).

The groups of participants mentioned earlier should undergo 17-hour training, during which, in addition to the basic knowledge on the physical basics of radiation, other topics such as general assumptions of radiological protection, permissible doses, and issues related to quality assurance programs in radiological protection are discussed. The latter issue seems to be important in the daily work of the invasive cardiology laboratory. That is because, in conjunction with the implementation of standard procedures, establishing rules that minimize exposure to ionizing radiation, registering doses where $K_{air,ref}$ exceeds 1.7 and 5 Gy, and managing patients exposed to such events or repeat procedures is of great importance for the correct and safe use of ionizing radiation. Indeed, constant improvement in qualifications in this area reduces late complications often unnoticed by invasive cardiologists, such as skin or hematological changes in treated patients, especially those who undergo multiple invasive cardiology procedures.

Patient radiological protection (PRP) training points may also be obtained by participating in other PRP-related training courses than those discussed earlier, at national or international scientific congresses, meetings, conferences, or symposia, or by giving lectures or presentations at national or international scientific congresses, meetings, conferences or symposia.

X-RAY PROTECTION FOR ECHOCARDIOGRAPHERS IN THE CATH LAB

Echocardiography, especially transesophageal (TEE), is an important monitoring tool for performing structural heart procedures in hemodynamic and hybrid rooms. The principles of radiological protection applicable to all staff working in them should also apply to imaging cardiologists to ensure their safety. In the literature, however, there are

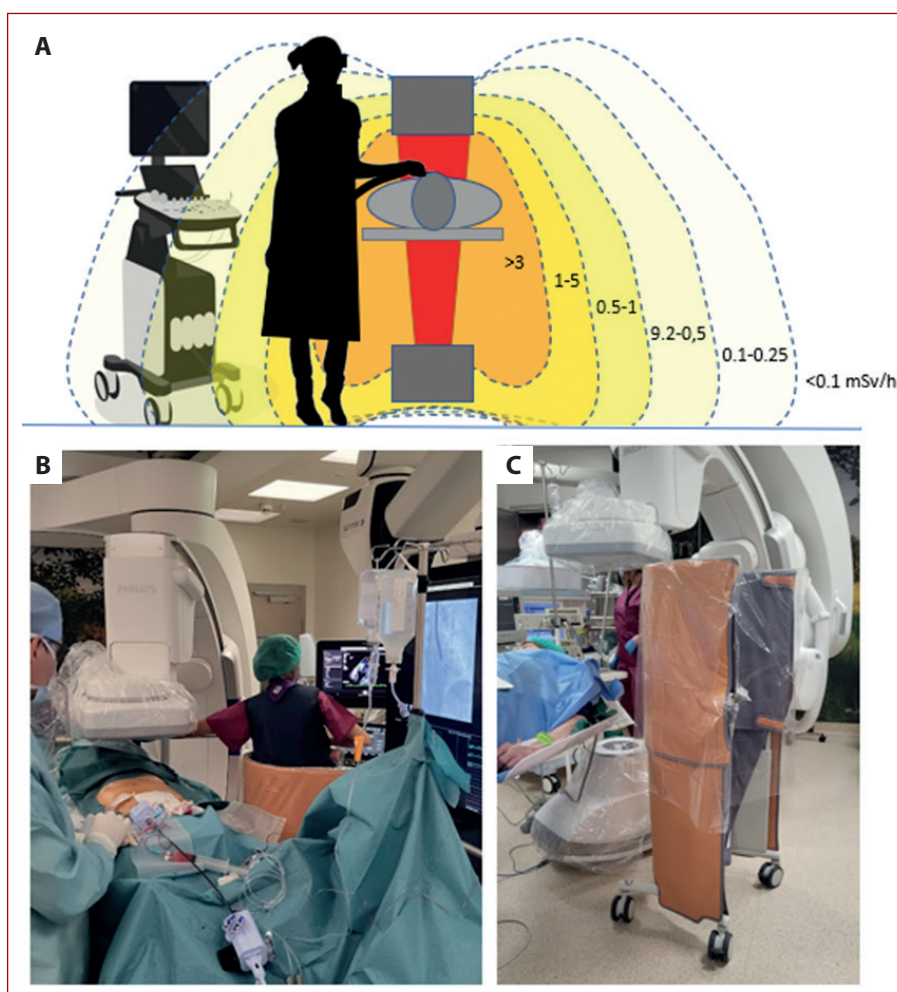


Figure 3. Approximate radiation power zones near the patient's head (A) (based on [87]). During surgery, the echocardiographer reaches into the patient's mouth to reposition the probe (B). A special mobile guard in the shape of a half-barrel with adjustable height (B, C)

scarce but disturbing data on X-ray doses affecting doctors performing ultrasound examinations during these procedures. These doses are comparable to those received by the patient and higher than the doses to which the invasive cardiologist is exposed.

This is due to several reasons. The first one is the echocardiographer's location near the patient's head, at a short distance from the radiation source. He/she often holds the probe in direct radiation, especially during transthoracic examinations or when manipulating the TEE probe (Figure 3A). The second problem involves difficult conditions for using standard lead shields. Unlike the interventional cardiologist, who stands near the patient's groin area and is protected by shields suspended under the table and the glass on the boom, the echocardiographer is located near the X-ray tube, where the use of such shields is more difficult because they can interfere with the moving C-arm. Some laboratories use special mobile shields between the patient and the TEE echocardiographer (Figure 3B-C), but this is uncommon. New solutions are also available on the market, like EggNest, which delivers protection to the entire team of the catheterization laboratory (as described

earlier). The lack of standard radiological protection for intra-procedural echocardiographers also applies to other European countries.

According to the regulations, all persons in the laboratory must comply with the principles of individual radiological protection: using lead aprons, shields for the thyroid gland, glasses, and newer technologies. Training in protection against radiation, dosimeters, and regular medical examinations are also necessary.

It is also advisable to collimate the X-ray beam and stop imaging when the echocardiographer's arm is in the radiation field (Figure 3B). Studies on echocardiographers' exposure demonstrate very different values of absorbed doses, whose direct comparison has limitations. The differences probably result from procedure types, fluoroscopy duration, quality of the fluoroscopy technique, type of radiological protection used, and the position of the echocardiographer in relation to the X-ray tube and the patient. However, they all indicate the highest X-ray exposure of the echocardiographer among cath lab personnel.

Another analysis of absorbed radiation doses for different parts of the body showed the highest values for the

echocardiographer, lower for the first operator, and lowest for the second operator. These differences were significant — the average radiation doses absorbed by the head were 2.5-fold higher, the arm – 6-fold larger, the hand – 3-fold larger, and the foot – 7-fold higher in echocardiographers compared to the first operators. Cumulative doses were also many times higher, e.g., cumulative dose for the head – echocardiographer 5.931 μSv , first operator – 2.109 μSv , second operator – 959 μSv ; cumulative dose for the hand – echocardiographer 20.720 μSv , first operator – 7.043 μSv , second operator – 4.629 μSv [5]. The highest radiation doses were associated with complex procedures, lower during left atrial appendage occlusion (LAAO), transcatheter edge-to-edge repair (TEER), and transcatheter aortic valve replacement, and lowest during atrial septal defect closure [82, 83].

In the publication comparing the individual dose equivalent during TEER and LAAO, the echocardiographer's exposure was also significantly higher than that of the invasive cardiologist: LAAO 10.6 vs. 3.5 μSv ; TEER 10.5 vs. 0.9 μSv , respectively. At the same time, over 25% of echocardiographers received a dose higher than 20 μSv , which is about 10-fold higher than the average dose received by an invasive cardiologist during a standard structural procedure [83].

It is important to relate these observations to the contemporary limits of the annual absorbed dose for the whole body — 5 rem (50 mSv) (according to the US Occupational Safety and Health Administration). This comparison indicates that the echocardiographer working in the operating room is at risk of exceeding this limit [83].

From a practical point of view, it is worth paying attention to the echocardiographer's location in relation to the X-ray tube. In the work of McNamara et al. [83], the echocardiographer stood at the height of the patient's head, facing the patient and the primary source of the radiation. In the study by Crowhurst et al. [13], the echocardiographer stood on the other side of the operating table in relation to the invasive cardiologist, with his/her back or side to the patient, at a 45° angle to the patient's head, which seems to be more advantageous. Reducing X-ray exposure of echocardiographers during structural procedures is extremely important and should be considered [84–86].

To summarise, regardless of general principles of protection against radiation, the specific rules related to TEE in the cath lab should be as follows:

- maximum distance of the echocardiographic device and its lateral position in relation to the X-ray tube (limitations: length of the TEE probe);
- limiting probe manipulation in the patient's mouth only to its occasional insertion and removal (other manipulations can be carried out using the probe handle located behind the cover and using the device's panel);
- use of optimal echocardiography imaging (including 3D) to reduce using X-ray radiation.

With the increasing number of structural procedures, echocardiographic monitoring and staff radiation exposure are becoming increasingly important. This also applies to anaesthesiologists and nurses, who periodically stay near the patient's head. Awareness of the significant problem of exposure to X-ray radiation should result in implementing preventive measures, including effective protection against radiation and active monitoring of side effects.

CONCLUSION

Team members of the catheterization laboratory constitute an occupational group that is particularly vulnerable to ionizing radiation with potentially serious health consequences. The growing number and complexity of interventional procedures engage physicians, nurses, technicians, and, more frequently, echocardiographers, anaesthesiologists, and medical physicists. All these groups require special attention, including law regulations, training, protection against radiation that utilizes modern angiographs and shields, monitoring, and treatment. Such a complex approach may significantly decrease their and patients' radiation-related health burden.

Supplementary material

Supplementary material is available at https://journals.viamedica.pl/polish_heart_journal.

Article information

Conflict of interest: None declared.

Funding: None.

Open access: This article is available in open access under Creative Commons Attribution-Non-Commercial-No Derivatives 4.0 International (CC BY-NC-ND 4.0) license, which allows downloading and sharing articles with others as long as they credit the authors and the publisher, but without permission to change them in any way or use them commercially. For commercial use, please contact the journal office at polishheartjournal@ptkardio.pl

REFERENCES

1. Andreassi MG, Piccaluga E, Guagliumi G, et al. Occupational health risks in cardiac catheterization laboratory workers. *Circ Cardiovasc Interv.* 2016; 9(4): e003273, doi: 10.1161/CIRCINTERVENTIONS.115.003273, indexed in Pubmed: 27072525.
2. Pedersen LN, Schiffer W, Mitchell JD, et al. Radiation-induced cardiac dysfunction: Practical implications. *Kardiol Pol.* 2022; 80(3): 256–265, doi: 10.33963/KP.a2022.0066, indexed in Pubmed: 35238396.
3. Zakeri F, Hirobe T, Akbari Noghabi K. Biological effects of low-dose ionizing radiation exposure on interventional cardiologists. *Occup Med (Lond).* 2010; 60(6): 464–469, doi: 10.1093/occmed/kqq062, indexed in Pubmed: 20519631.
4. Halliday D, Resnick R, Walker J. *Fundamentals of Physics (part 5)*. John Wiley & Sons 2005.
5. Łobodziec W. *Fundamentals of the physics of ionizing radiation for the use of radiotherapy and imaging diagnostics*. Publishing house of the University of Rzeszów, Rzeszów 2016.
6. *Technical Reports Series No. 457, Dosimetry in Diagnostic Radiology: An International Code of Practice*. Vienna, 2007.
7. *The 2007 Recommendations of the International Commission on Radiological Protection ICRP Publication 103* 2007.
8. Announcement of the Marshal of the Sejm of the Republic of Poland of May 11, 2023 on the publication of the consolidated text of the Atomic Law. *Dz. U.* 2023 poz. 1173.

9. Kidoń J. Assessment of ionizing radiation doses for staff and patients in cardiology and interventional radiology procedures using dosimetric systems [Doctoral dissertation, Medical University of Silesia in Katowice]. Repository of the Medical University of Silesia in Katowice, 2020.
10. Occupational Radiological Protection in Interventional Procedures, ICRP Publication 139 2018.
11. Hirshfeld JW, Ferrari VA, Bengel FM, et al. 2018 ACC/HRS/NASCI/SCAI/SCCT expert consensus document on optimal use of ionizing radiation in cardiovascular imaging: Best practices for safety and effectiveness: A report of the American College of Cardiology task force on expert consensus decision pathways. *J Am Coll Cardiol*. 2018; 71(24): e283–e351, doi: [10.1016/j.jacc.2018.02.016](https://doi.org/10.1016/j.jacc.2018.02.016), indexed in Pubmed: 29729877.
12. Lie ØØ, Paulsen GU, Wøhni T. Assessment of effective dose and dose to the lens of the eye for the interventional cardiologist. *Radiat Prot Dosimetry*. 2008; 132(3): 313–318, doi: [10.1093/rpd/ncn296](https://doi.org/10.1093/rpd/ncn296), indexed in Pubmed: 19056809.
13. Crowhurst JA, Scalia GM, Whitby M, et al. Radiation exposure of operators performing transesophageal echocardiography during percutaneous structural cardiac interventions. *J Am Coll Cardiol*. 2018; 71(11): 1246–1254, doi: [10.1016/j.jacc.2018.01.024](https://doi.org/10.1016/j.jacc.2018.01.024), indexed in Pubmed: 29544609.
14. Giordano BD, Baumhauer JF, Morgan TL, et al. Cervical spine imaging using standard C-arm fluoroscopy: Patient and surgeon exposure to ionizing radiation. *Spine (Phila Pa 1976)*. 2008; 33(18): 1970–1976, doi: [10.1097/BRS.0b013e31817e69b7](https://doi.org/10.1097/BRS.0b013e31817e69b7), indexed in Pubmed: 18665022.
15. Giordano BD, Baumhauer JF, Morgan TL, et al. Patient and surgeon radiation exposure: comparison of standard and mini-C-arm fluoroscopy. *J Bone Joint Surg Am*. 2009; 91(2): 297–304, doi: [10.2106/JBJS.H.00407](https://doi.org/10.2106/JBJS.H.00407), indexed in Pubmed: 19181973.
16. Gerber TC, Carr JJ, Arai AE, et al. Ionizing radiation in cardiac imaging: a science advisory from the American Heart Association Committee on Cardiac Imaging of the Council on Clinical Cardiology and Committee on Cardiovascular Imaging and Intervention of the Council on Cardiovascular Radiology and Intervention. *Circulation*. 2009; 119(7): 1056–1065, doi: [10.1161/CIRCULATIONAHA.108.191650](https://doi.org/10.1161/CIRCULATIONAHA.108.191650), indexed in Pubmed: 19188512.
17. Zielinski JM, Garner MJ, Band PR, et al. Health outcomes of low-dose ionizing radiation exposure among medical workers: A cohort study of the Canadian national dose registry of radiation workers. *Int J Occup Med Environ Health*. 2009; 22(2): 149–156, doi: [10.2478/v10001-009-0010-y](https://doi.org/10.2478/v10001-009-0010-y), indexed in Pubmed: 19546093.
18. Yoshinaga S, Mabuchi K, Sigurdson AJ, et al. Cancer risks among radiologists and radiologic technologists: Review of epidemiologic studies. *Radiology*. 2004; 233(2): 313–321, doi: [10.1148/radiol.2332031119](https://doi.org/10.1148/radiol.2332031119), indexed in Pubmed: 15375227.
19. Blakely EA, Kleiman NJ, Neriishi K, et al. Radiation cataractogenesis: Epidemiology and biology. *Radiat Res*. 2010; 173(5): 709–717, doi: [10.1667/RRXX19.1](https://doi.org/10.1667/RRXX19.1), indexed in Pubmed: 20426671.
20. Ciraj-Bjelac O, Rehani MM, Sim KH, et al. Risk for radiation-induced cataract for staff in interventional cardiology: is there reason for concern? *Catheter Cardiovasc Interv*. 2010; 76(6): 826–834, doi: [10.1002/ccd.22670](https://doi.org/10.1002/ccd.22670), indexed in Pubmed: 20549683.
21. Chodick G, Bekiroglu N, Hauptmann M, et al. Risk of cataract after exposure to low doses of ionizing radiation: A 20-year prospective cohort study among US radiologic technologists. *Am J Epidemiol*. 2008; 168(6): 620–631, doi: [10.1093/aje/kwn171](https://doi.org/10.1093/aje/kwn171), indexed in Pubmed: 18664497.
22. Khafaji M, Ashour TM, Mozahim NF, et al. Measurement of occupational eye and thyroid radiation doses in pediatric interventional cardiologists at a tertiary hospital. *Cureus*. 2023; 15(9): e44894, doi: [10.7759/cureus.44894](https://doi.org/10.7759/cureus.44894), indexed in Pubmed: 37814769.
23. Mohan AK, Hauptmann M, Freedman DM, et al. Cancer and other causes of mortality among radiologic technologists in the United States. *Int J Cancer*. 2003; 103(2): 259–267, doi: [10.1002/ijc.10811](https://doi.org/10.1002/ijc.10811), indexed in Pubmed: 12455042.
24. Wang JX, Zhang LA, Li BX, et al. Cancer incidence and risk estimation among medical x-ray workers in China, 1950–1995. *Health Phys*. 2002; 82(4): 455–466, doi: [10.1097/00004032-200204000-00004](https://doi.org/10.1097/00004032-200204000-00004), indexed in Pubmed: 11906134.
25. Doody MM, Freedman DM, Alexander BH, et al. Breast cancer incidence in U.S. radiologic technologists. *Cancer*. 2006; 106(12): 2707–2715, doi: [10.1002/cncr.21876](https://doi.org/10.1002/cncr.21876), indexed in Pubmed: 16639729.
26. Bonassi S, Forni A, Bigatti P, et al. Chromosome aberrations in hospital workers: Evidence from surveillance studies in Italy (1963–1993). *Am J Ind Med*. 1997; 31(3): 353–360, doi: [10.1002/\(sici\)1097-0274\(199703\)31:3<353::aid-ajim12>3.0.co;2-#](https://doi.org/10.1002/(sici)1097-0274(199703)31:3<353::aid-ajim12>3.0.co;2-#), indexed in Pubmed: 9055959.
27. Engin AB, Ergun MA, Yurtcu E, et al. Effect of ionizing radiation on the pteridine metabolic pathway and evaluation of its cytotoxicity in exposed hospital staff. *Mutat Res*. 2005; 585(1–2): 184–192, doi: [10.1016/j.mrgen-tox.2005.05.005](https://doi.org/10.1016/j.mrgen-tox.2005.05.005), indexed in Pubmed: 15998597.
28. Scarpato R, Antonelli A, Ballardin M, et al. Analysis of chromosome damage in circulating lymphocytes of radiological workers affected by thyroid nodules. *Mutat Res*. 2006; 606(1–2): 21–26, doi: [10.1016/j.mrgen-tox.2006.02.012](https://doi.org/10.1016/j.mrgen-tox.2006.02.012), indexed in Pubmed: 16713331.
29. Gaetani S, Monaco F, Bracci M, et al. DNA damage response in workers exposed to low-dose ionising radiation. *Occup Environ Med*. 2018; 75(10): 724–729, doi: [10.1136/oemed-2018-105094](https://doi.org/10.1136/oemed-2018-105094), indexed in Pubmed: 30087158.
30. Cardoso RS, Takahashi-Hyodo S, Peitl P, et al. Evaluation of chromosomal aberrations, micronuclei, and sister chromatid exchanges in hospital workers chronically exposed to ionizing radiation. *Teratog Carcinog Mutagen*. 2001; 21(6): 431–439, doi: [10.1002/tcm.1030](https://doi.org/10.1002/tcm.1030), indexed in Pubmed: 11746256.
31. Fenech M, Perepetskaya G, Mikhalevich L. A more comprehensive application of the micronucleus technique for biomonitoring of genetic damage rates in human populations—experiences from the Chernobyl catastrophe. *Environ Mol Mutagen*. 1997; 30(2): 112–118, indexed in Pubmed: 9329635.
32. Bouraoui S, Mougou S, Drira A, et al. A cytogenetic approach to the effects of low levels of ionizing radiation (IR) on the exposed Tunisian hospital workers. *Int J Occup Med Environ Health*. 2013; 26(1): 144–154, doi: [10.2478/s13382-013-0084-4](https://doi.org/10.2478/s13382-013-0084-4), indexed in Pubmed: 23559140.
33. Regulation of the Minister of Health of September 13, 2021, on minimum requirements for health care units conducting activities involving exposure for medical purposes, consisting of providing health services in the field of X-ray diagnostics, interventional radiology, or diagnostics related to the administration of radiopharmaceutical products to patients. *Dz.U.* 2021 poz. 1725.
34. Notice of the Minister of Health of November 10, 2015 regarding the announcement of a list of standard radiological procedures in the field of radiology — diagnostic imaging and interventional radiology.
35. Regulation of The Council of Ministers of November 30, 2020, on the protection against ionizing radiation of external workers exposed at work in a controlled or supervised area. *Dz.U.* 2020 poz. 2313.
36. Regulation of the Council of Ministers of March 5, 2021 on radiological protection inspectors. *Dz.U.* 2021 poz. 640.
37. Balter S, Hopewell JW, Miller DL, et al. Fluoroscopically guided interventional procedures: A review of radiation effects on patients' skin and hair. *Radiology*. 2010; 254(2): 326–341, doi: [10.1148/radiol.2542082312](https://doi.org/10.1148/radiol.2542082312), indexed in Pubmed: 20093507.
38. Jaszke W, Schmutz M, Trianni A, et al. Radiation-induced skin injuries to patients: What the interventional radiologist needs to know. *Cardiovasc Intervent Radiol*. 2017; 40(8): 1131–1140, doi: [10.1007/s00270-017-1674-5](https://doi.org/10.1007/s00270-017-1674-5), indexed in Pubmed: 28497187.
39. McParland BJ. Entrance skin dose estimates derived from dose-area product measurements in interventional radiological procedures. *Br J Radiol*. 1998; 71(852): 1288–1295, doi: [10.1259/bjr.71.852.10319003](https://doi.org/10.1259/bjr.71.852.10319003), indexed in Pubmed: 10319003.
40. Notice of the Minister of Health of April 3, 2017, on the announcement of the uniform text of the regulation of the Minister of Health on the conditions for the safe use of ionizing radiation for all types of medical exposure. *Dz.U.* 2017 poz. 884.
41. Regulation of The Minister of Health of December 13, 2022 on the categories and criteria for qualifying unintentional and accidental exposures, necessary actions in the health care unit after their occurrence, as well as the scope of information included in the Central Register of Unintentional and Accidental Exposures. *Dz.U.* 2022 poz. 2700.
42. Regulation of the Minister of Health of January 11, 2023, on the conditions for the safe use of ionizing radiation for all types of medical exposure. *Dz.U.* 2023 poz. 195.
43. National Council on Radiation Protection and Measurements. Radiation dose management for fluoroscopically guided interventional medical

- procedures. Bethesda, Md.: National Council on Radiation Protection and Measurements; 2011. xii, 325 p. p.
44. Sánchez R, Vañó E, Fernández Soto JM, et al. Updating national diagnostic reference levels for interventional cardiology and methodological aspects. *Phys Med*. 2020; 70: 169–175, doi: [10.1016/j.ejmp.2020.01.014](https://doi.org/10.1016/j.ejmp.2020.01.014), indexed in Pubmed: [32032801](https://pubmed.ncbi.nlm.nih.gov/32032801/).
 45. Rizk C, Fares G, Vanhavere F, et al. Diagnostic reference levels, deterministic and stochastic risks in pediatric interventional cardiology procedures. *Health Phys*. 2020; 118(1): 85–95, doi: [10.1097/HP.0000000000001114](https://doi.org/10.1097/HP.0000000000001114), indexed in Pubmed: [31764423](https://pubmed.ncbi.nlm.nih.gov/31764423/).
 46. Trueb PR, Aroua A, Stuessi A, Samara E, Treier R, Verdun FR, et al., editors. Diagnostic Reference Levels in Cardiology and Interventional Radiology. World Congress on Medical Physics and Biomedical Engineering Munich, Germany, September 7-12, 2009.
 47. Samara ET, Aroua A, De Palma R, et al. An audit of diagnostic reference levels in interventional cardiology and radiology: Are there differences between academic and non-academic centres? *Radiat Prot Dosimetry*. 2012; 148(1): 74–82, doi: [10.1093/rpd/ncq600](https://doi.org/10.1093/rpd/ncq600), indexed in Pubmed: [21335331](https://pubmed.ncbi.nlm.nih.gov/21335331/).
 48. Ruiz-Cruces R, Vano E, Carrera-Magariño F, et al. Diagnostic reference levels and complexity indices in interventional radiology: A national programme. *Eur Radiol*. 2016; 26(12): 4268–4276, doi: [10.1007/s00330-016-4334-2](https://doi.org/10.1007/s00330-016-4334-2), indexed in Pubmed: [27384609](https://pubmed.ncbi.nlm.nih.gov/27384609/).
 49. Kidoń J, Polaczek-Grelík K, Wojciuch L. Local diagnostic reference levels and effective doses: single institution levels for interventional cardiology procedures for adult patients. *Pol J Med Phys Eng*. 2022; 28(2): 77–83, doi: [10.2478/pjmpe-2022-0009](https://doi.org/10.2478/pjmpe-2022-0009).
 50. Regulation of the Minister of Health of December 6, 2022 on diagnostic reference levels. *Dz.U.* 2022 poz. 2626.
 51. Regulation of the Minister of Health of March 8, 2023 on special protection of certain categories of people in relation to medical exposure during diagnostic tests, procedures and treatment. *Dz.U.* 2023 poz. 576.
 52. Marx MV, Niklason L, Mauger EA. Occupational radiation exposure to interventional radiologists: a prospective study. *J Vasc Interv Radiol*. 1992; 3(4): 597–606, doi: [10.1016/s1051-0443\(92\)72903-0](https://doi.org/10.1016/s1051-0443(92)72903-0), indexed in Pubmed: [1446120](https://pubmed.ncbi.nlm.nih.gov/1446120/).
 53. Miller DL, Martin CJ, Rehani MM. The mandate and work of ICRP Committee 3 on radiological protection in medicine. *Ann ICRP*. 2018; 47(3–4): 142–151, doi: [10.1177/0146645318756249](https://doi.org/10.1177/0146645318756249), indexed in Pubmed: [29714065](https://pubmed.ncbi.nlm.nih.gov/29714065/).
 54. Sans-Merce M, Ruiz N, Barth I, et al. Recommendations to reduce hand exposure for standard nuclear medicine procedures. *Radiation Measurements*. 2011; 46(11): 1330–1333, doi: [10.1016/j.radmeas.2011.07.011](https://doi.org/10.1016/j.radmeas.2011.07.011).
 55. Kidoń J, Polaczek-Grelík K, Żurek P, et al. Exposure of the eye lens and brain for interventional cardiology staff. *Postępy Kardiologii Interwencyjnej*. 2021; 17(3): 298–304, doi: [10.5114/aic.2021.109576](https://doi.org/10.5114/aic.2021.109576), indexed in Pubmed: [34819966](https://pubmed.ncbi.nlm.nih.gov/34819966/).
 56. Wagner LK, Mulhern OR. Radiation-attenuating surgical gloves: effects of scatter and secondary electron production. *Radiology*. 1996; 200(1): 45–48, doi: [10.1148/radiology.200.1.8657942](https://doi.org/10.1148/radiology.200.1.8657942), indexed in Pubmed: [8657942](https://pubmed.ncbi.nlm.nih.gov/8657942/).
 57. Martin CJ. A review of radiology staff doses and dose monitoring requirements. *Radiat Prot Dosimetry*. 2009; 136(3): 140–157, doi: [10.1093/rpd/ncp168](https://doi.org/10.1093/rpd/ncp168), indexed in Pubmed: [19759087](https://pubmed.ncbi.nlm.nih.gov/19759087/).
 58. Suryadevara R, Brown ED, Green SM, et al. A randomized controlled trial to assess operator radiation exposure from cardiac catheterization procedures using RAD BOARD® with standard pelvic shielding versus standard pelvic shielding alone. *Catheter Cardiovasc Interv*. 2020; 95(1): 83–88, doi: [10.1002/ccd.28190](https://doi.org/10.1002/ccd.28190), indexed in Pubmed: [30866175](https://pubmed.ncbi.nlm.nih.gov/30866175/).
 59. Sciahbasi A, Sarandrea A, Rigattieri S, et al. Extended protective shield under table to reduce operator radiation dose in percutaneous coronary procedures. *Circ Cardiovasc Interv*. 2019; 12(2): e007586, doi: [10.1161/CIRCINTERVENTIONS.118.007586](https://doi.org/10.1161/CIRCINTERVENTIONS.118.007586), indexed in Pubmed: [30732471](https://pubmed.ncbi.nlm.nih.gov/30732471/).
 60. Shortt CP, Al-Hashimi H, Malone L, et al. Staff radiation doses to the lower extremities in interventional radiology. *Cardiovasc Intervent Radiol*. 2007; 30(6): 1206–1209, doi: [10.1007/s00270-007-9071-0](https://doi.org/10.1007/s00270-007-9071-0), indexed in Pubmed: [17533541](https://pubmed.ncbi.nlm.nih.gov/17533541/).
 61. King JN, Champlin AM, Kelsey CA, et al. Using a sterile disposable protective surgical drape for reduction of radiation exposure to interventionalists. *AJR Am J Roentgenol*. 2002; 178(1): 153–157, doi: [10.2214/ajr.178.1.1780153](https://doi.org/10.2214/ajr.178.1.1780153), indexed in Pubmed: [11756110](https://pubmed.ncbi.nlm.nih.gov/11756110/).
 62. Musallam A, Volis I, Dadaev S, et al. A randomized study comparing the use of a pelvic lead shield during trans-radial interventions: Threefold decrease in radiation to the operator but double exposure to the patient. *Catheter Cardiovasc Interv*. 2015; 85(7): 1164–1170, doi: [10.1002/ccd.25777](https://doi.org/10.1002/ccd.25777), indexed in Pubmed: [25510441](https://pubmed.ncbi.nlm.nih.gov/25510441/).
 63. Jones MA, Cocker M, Khiani R, et al. The benefits of using a bismuth-containing, radiation-absorbing drape in cardiac resynchronization implant procedures. *Pacing Clin Electrophysiol*. 2014; 37(7): 828–833, doi: [10.1111/pace.12349](https://doi.org/10.1111/pace.12349), indexed in Pubmed: [24697669](https://pubmed.ncbi.nlm.nih.gov/24697669/).
 64. Vlastra W, Delewi R, Sjaun KD, et al. Efficacy of the RADPAD protection drape in reducing operators' radiation exposure in the catheterization laboratory: A sham-controlled randomized trial. *Circ Cardiovasc Interv*. 2017; 10(11): e006058, doi: [10.1161/CIRCINTERVENTIONS.117.006058](https://doi.org/10.1161/CIRCINTERVENTIONS.117.006058), indexed in Pubmed: [29089313](https://pubmed.ncbi.nlm.nih.gov/29089313/).
 65. Shah P, Khanna R, Kapoor A, et al. Efficacy of RADPAD protection drape in reducing radiation exposure in the catheterization laboratory—First Indian study. *Indian Heart J*. 2018; 70 Suppl 3(Suppl 3): S265–S268, doi: [10.1016/j.ihj.2018.03.008](https://doi.org/10.1016/j.ihj.2018.03.008), indexed in Pubmed: [30595271](https://pubmed.ncbi.nlm.nih.gov/30595271/).
 66. Kherad B, Jerichow T, Blaschke F, et al. Efficacy of RADPAD protective drape during coronary angiography. *Herz*. 2018; 43(4): 310–314, doi: [10.1007/s00059-017-4560-7](https://doi.org/10.1007/s00059-017-4560-7), indexed in Pubmed: [28389764](https://pubmed.ncbi.nlm.nih.gov/28389764/).
 67. Dehmer GJ. Occupational hazards for interventional cardiologists. *Catheter Cardiovasc Interv*. 2006; 68(6): 974–976, doi: [10.1002/ccd.21004](https://doi.org/10.1002/ccd.21004), indexed in Pubmed: [17091487](https://pubmed.ncbi.nlm.nih.gov/17091487/).
 68. Goldstein JA, Balter S, Cowley M, et al. Occupational hazards of interventional cardiologists: prevalence of orthopedic health problems in contemporary practice. *Catheter Cardiovasc Interv*. 2004; 63(4): 407–411, doi: [10.1002/ccd.20201](https://doi.org/10.1002/ccd.20201), indexed in Pubmed: [15558765](https://pubmed.ncbi.nlm.nih.gov/15558765/).
 69. Marichal DA, Anwar T, Kirsch D, et al. Comparison of a suspended radiation protection system versus standard lead apron for radiation exposure of a simulated interventionalist. *J Vasc Interv Radiol*. 2011; 22(4): 437–442, doi: [10.1016/j.jvir.2010.12.016](https://doi.org/10.1016/j.jvir.2010.12.016), indexed in Pubmed: [21354818](https://pubmed.ncbi.nlm.nih.gov/21354818/).
 70. Katsarou M, Zwiebel B, Vogler J, et al. StemRad MD, an exoskeleton-based radiation protection against radiation system, reduces ergonomic posture risk based on a prospective observational study. *J Endovasc Ther*. 2024; 31(4): 668–674, doi: [10.1177/15266028231160661](https://doi.org/10.1177/15266028231160661), indexed in Pubmed: [36942629](https://pubmed.ncbi.nlm.nih.gov/36942629/).
 71. Brilakis ES. Innovations in radiation safety during cardiovascular catheterization. *Circulation*. 2018; 137(13): 1317–1319, doi: [10.1161/CIRCULATIONAHA.117.032808](https://doi.org/10.1161/CIRCULATIONAHA.117.032808), indexed in Pubmed: [29581362](https://pubmed.ncbi.nlm.nih.gov/29581362/).
 72. Laish-Farkash A, Harari E, Finkelstein A, et al. A novel robotic radiation shielding device for interventional cardiology procedures. *EuroIntervention*. 2022; 18(3): 262–266, doi: [10.4244/EIJ-D-21-00577](https://doi.org/10.4244/EIJ-D-21-00577), indexed in Pubmed: [35094972](https://pubmed.ncbi.nlm.nih.gov/35094972/).
 73. Dębski MA, Kruk M, Bujak S, et al. Benefits of the selective invasive strategy guided by CTA and CTA-derived fractional flow reserve in patients with coronary artery disease. *Kardiologia Pol*. 2023; 81(3): 252–258, doi: [10.33963/KP.a2022.0264](https://doi.org/10.33963/KP.a2022.0264), indexed in Pubmed: [36446067](https://pubmed.ncbi.nlm.nih.gov/36446067/).
 74. Chakravarti J, Rao SV. Robotic assisted percutaneous coronary intervention: hype or hope? *J Am Heart Assoc*. 2019; 8(13): e012743, doi: [10.1161/JAHA.119.012743](https://doi.org/10.1161/JAHA.119.012743), indexed in Pubmed: [31257969](https://pubmed.ncbi.nlm.nih.gov/31257969/).
 75. Smitson CC, Ang L, Pourdjabbar A, et al. Safety and feasibility of a novel, second-generation robotic-assisted system for percutaneous coronary intervention: First-in-human report. *J Invasive Cardiol*. 2018; 30(4): 152–156, indexed in Pubmed: [29335386](https://pubmed.ncbi.nlm.nih.gov/29335386/).
 76. Kagiyama K, Mitsutake Y, Ueno T, et al. Successful introduction of robotic-assisted percutaneous coronary intervention system into Japanese clinical practice: A first-year survey at single center. *Heart Vessels*. 2021; 36(7): 955–964, doi: [10.1007/s00380-021-01782-6](https://doi.org/10.1007/s00380-021-01782-6), indexed in Pubmed: [33502572](https://pubmed.ncbi.nlm.nih.gov/33502572/).
 77. Walters D, Reeves RR, Patel M, et al. Complex robotic compared to manual coronary interventions: 6- and 12-month outcomes. *Catheter Cardiovasc Interv*. 2019; 93(4): 613–617, doi: [10.1002/ccd.27867](https://doi.org/10.1002/ccd.27867), indexed in Pubmed: [30456889](https://pubmed.ncbi.nlm.nih.gov/30456889/).
 78. Harrison J, Ang L, Naghi J, et al. Robotically-assisted percutaneous coronary intervention: Reasons for partial manual assistance or manual conversion. *Cardiovasc Revasc Med*. 2018; 19(5 Pt A): 526–531, doi: [10.1016/j.carrev.2017.11.003](https://doi.org/10.1016/j.carrev.2017.11.003), indexed in Pubmed: [29221959](https://pubmed.ncbi.nlm.nih.gov/29221959/).
 79. Wegermann ZK, Swaminathan RV, Rao SV. Cath lab robotics: Paradigm change in interventional cardiology? *Curr Cardiol Rep*. 2019; 21(10): 119, doi: [10.1007/s11886-019-1218-5](https://doi.org/10.1007/s11886-019-1218-5), indexed in Pubmed: [31473815](https://pubmed.ncbi.nlm.nih.gov/31473815/).

80. Council Directive 2013/59/Euratom laying down basic safety standards for protection against the dangers arising from exposure to ionising radiation, and repealing Directives 89/618/Euratom, 90/641/Euratom, 96/29/Euratom, 97/43/Euratom and 2003/122/Euratom.
81. Regulation of the Minister of Health of March 6, 2020 on training in the field of radiation protection of patient. Dz.U. 2020 poz. 390.
82. Salaun E, Carles S, Bigand E, et al. High radiation exposure of the imaging specialist during structural heart interventions with echocardiographic guidance. *JACC Cardiovasc Interv.* 2017; 10(6): 626–627, doi: [10.1016/j.jcin.2017.01.016](https://doi.org/10.1016/j.jcin.2017.01.016), indexed in Pubmed: [28335903](https://pubmed.ncbi.nlm.nih.gov/28335903/).
83. McNamara DA, Chopra R, Decker JM, et al. Comparison of radiation exposure among interventional echocardiographers, interventional cardiologists, and sonographers during percutaneous structural heart interventions. *JAMA Netw Open.* 2022; 5(7): e2220597, doi: [10.1001/jamanetworkopen.2022.20597](https://doi.org/10.1001/jamanetworkopen.2022.20597), indexed in Pubmed: [35797046](https://pubmed.ncbi.nlm.nih.gov/35797046/).
84. Salaun E, Carles S, Bigand E, et al. High radiation exposure of the imaging specialist during structural heart interventions with echocardiographic guidance. *JACC Cardiovasc Interv.* 2017; 10(6): 626–627, doi: [10.1016/j.jcin.2017.01.016](https://doi.org/10.1016/j.jcin.2017.01.016), indexed in Pubmed: [28335903](https://pubmed.ncbi.nlm.nih.gov/28335903/).
85. Corrigan FE, Hall MJ, Iturbe JM, et al. Radioprotective strategies for interventional echocardiographers during structural heart interventions. *Catheter Cardiovasc Interv.* 2019; 93(2): 356–361, doi: [10.1002/ccd.27843](https://doi.org/10.1002/ccd.27843), indexed in Pubmed: [30196578](https://pubmed.ncbi.nlm.nih.gov/30196578/).
86. Jone PN, Zablah JE, Burkett DA, et al. Three-dimensional echocardiographic guidance of right heart catheterization decreases radiation exposure in atrial septal defect closures. *J Am Soc Echocardiogr.* 2018; 31(9): 1044–1049, doi: [10.1016/j.echo.2018.04.016](https://doi.org/10.1016/j.echo.2018.04.016), indexed in Pubmed: [29958759](https://pubmed.ncbi.nlm.nih.gov/29958759/).
87. Wilson-Stewart K, Shanahan M, Fontanarosa D, et al. Occupational radiation exposure to nursing staff during cardiovascular fluoroscopic procedures: A review of the literature. *J Appl Clin Med Phys.* 2018; 19(6): 282–297, doi: [10.1002/acm2.12461](https://doi.org/10.1002/acm2.12461), indexed in Pubmed: [30294978](https://pubmed.ncbi.nlm.nih.gov/30294978/).