

Supplementary material

Wojakowski W, Smolka G, Piazza N, et al. Transseptal implantation of the HighLife self-expandable mitral valve in a patient with severe secondary mitral regurgitation and heart failure. Kardiol Pol. 2021.

Please note that the journal is not responsible for the scientific accuracy or functionality of any supplementary material submitted by the authors. Any queries (except missing content) should be directed to the corresponding author of the article.

Figure S1. Preprocedural transoesophageal imaging showing mitral regurgitation

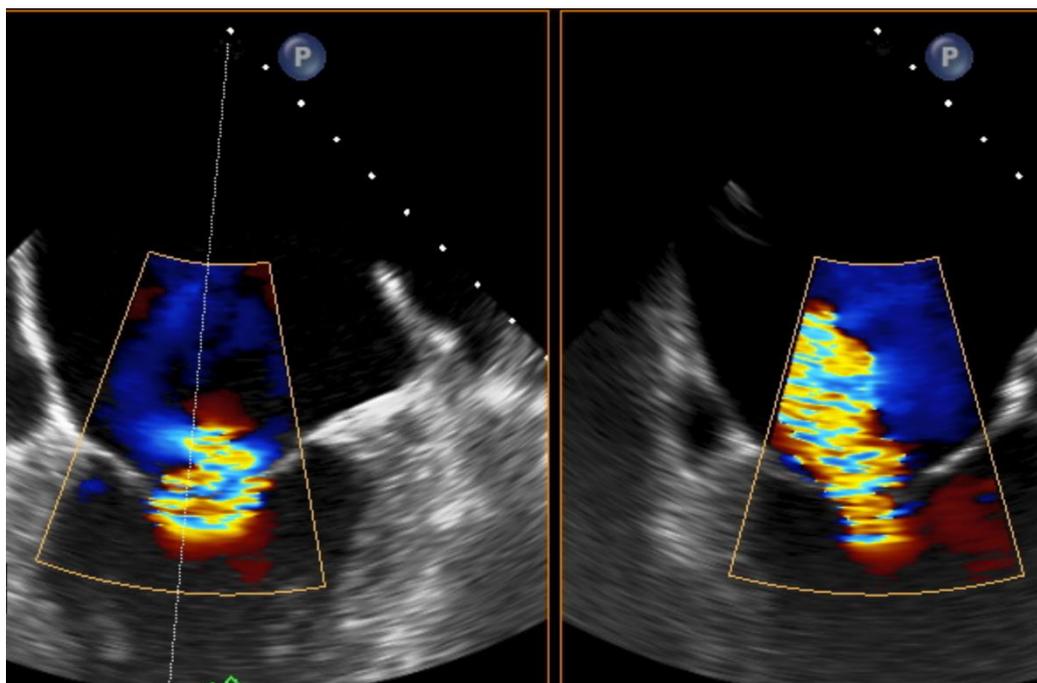


Figure S2. Postprocedural transoesophageal imaging

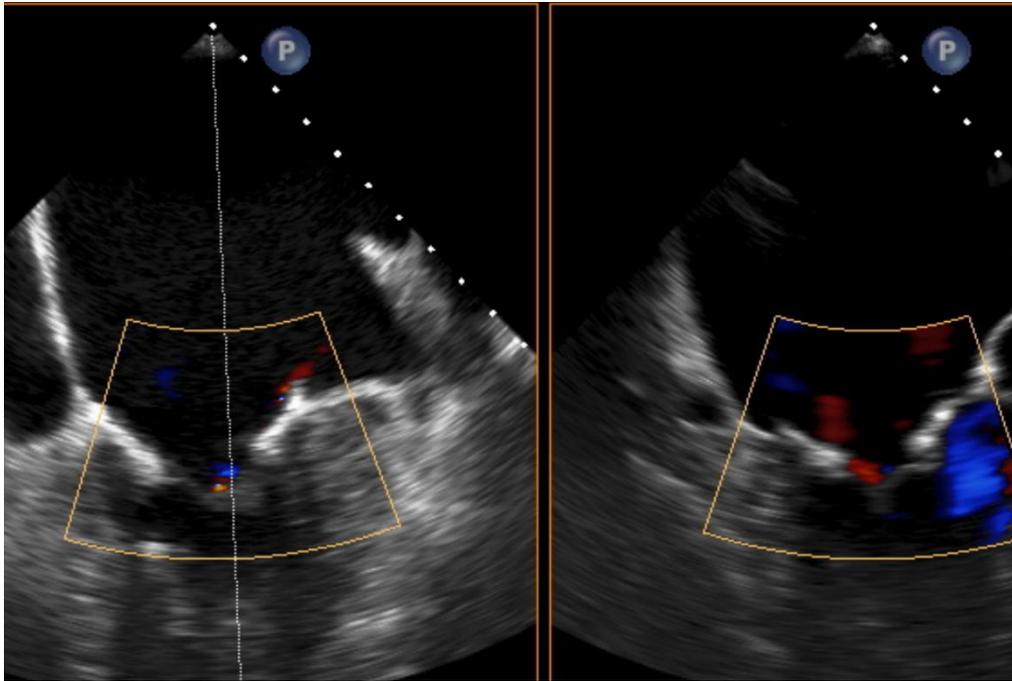


Figure S3. Persistent iatrogenic ASD

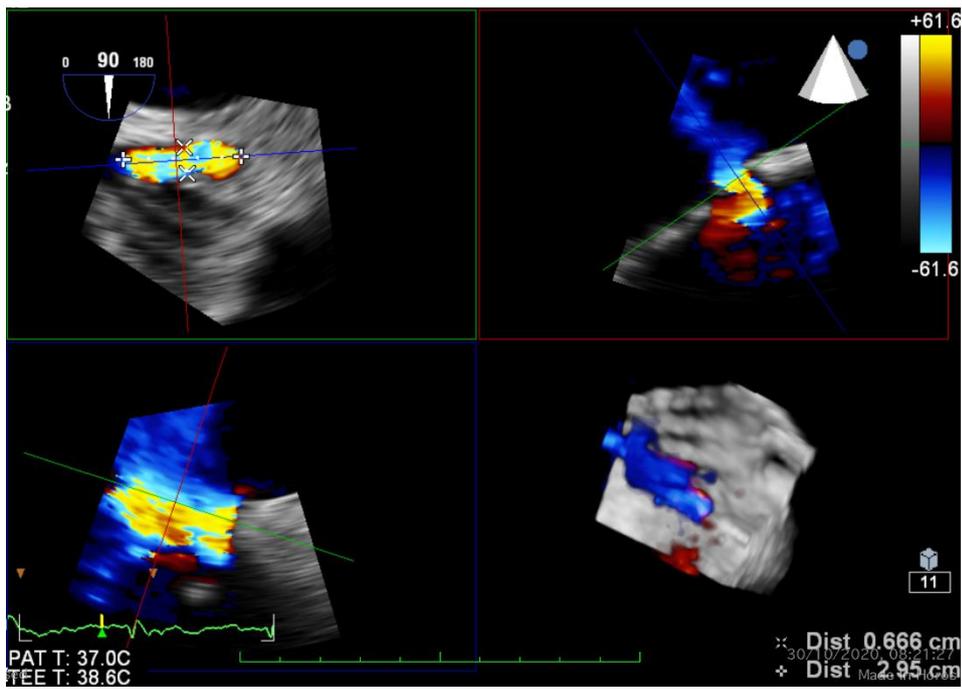


Figure S4. 3D transoesophageal imaging of the HighLife valve and ASD occluder

