

Supplementary material

Kocańda S, Stankiewicz A, Mitrosz M, et al. The standardization of the aortic valve sparing procedure allows to introduce the new surgical technique with good early results: Retrospective analysis. Pol Heart J. 2024.

Please note that the journal is not responsible for the scientific accuracy or functionality of any supplementary material submitted by the authors. Any queries (except missing content) should be directed to the corresponding author of the article.

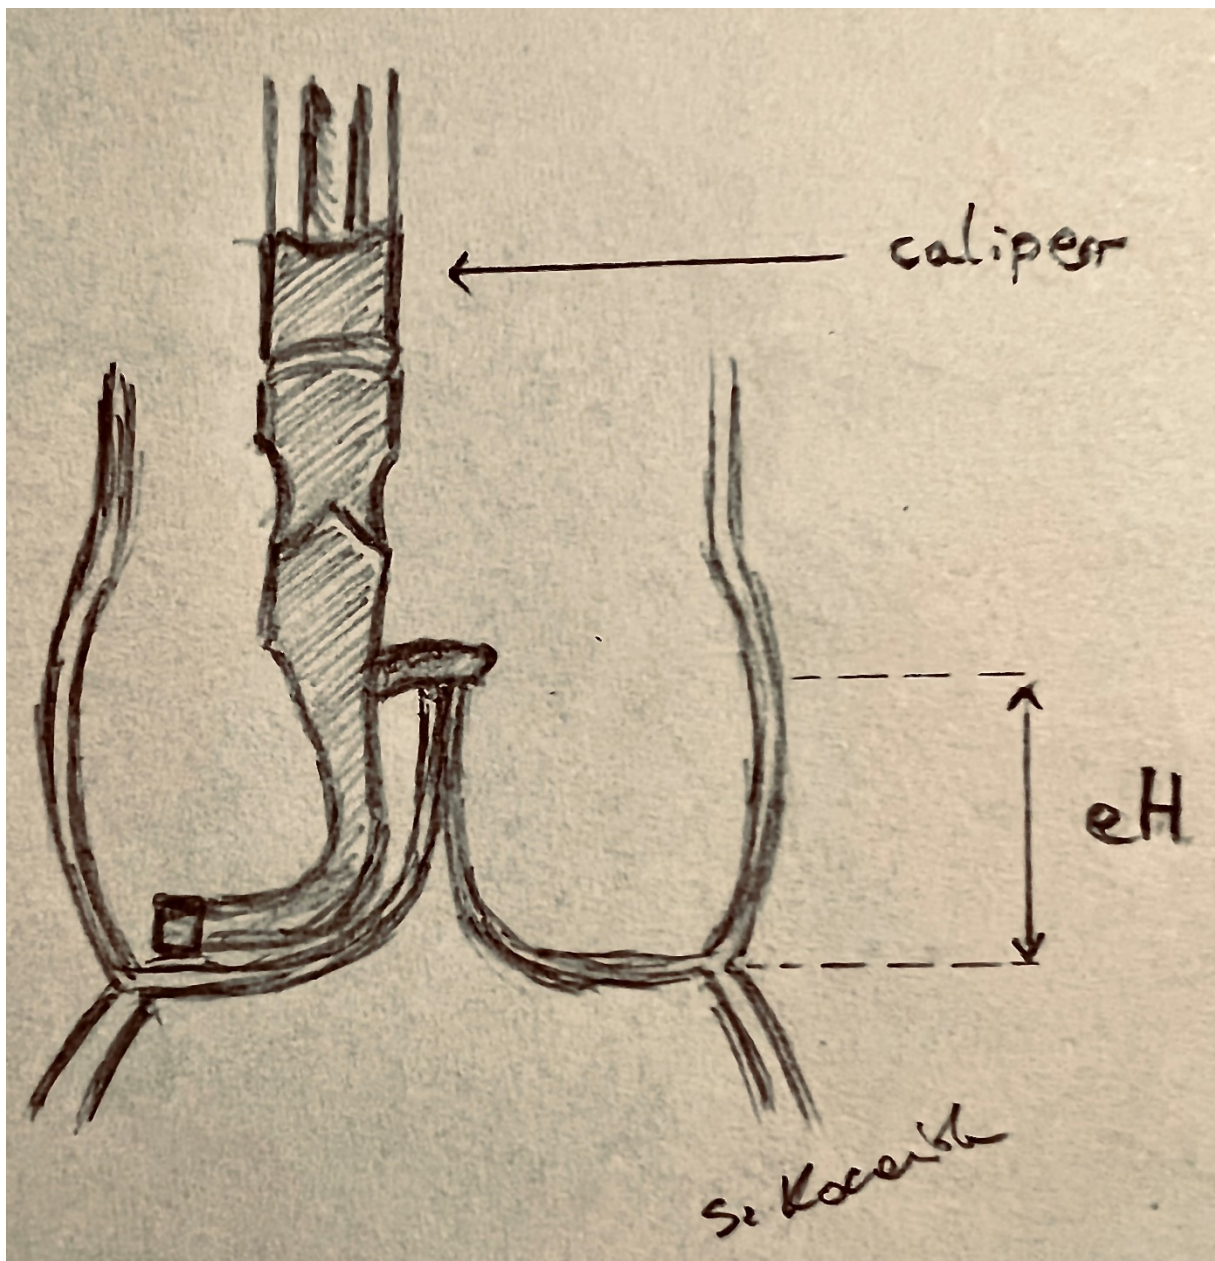


Figure S1. Schäfers caliper

Abbreviation: eH, effective height

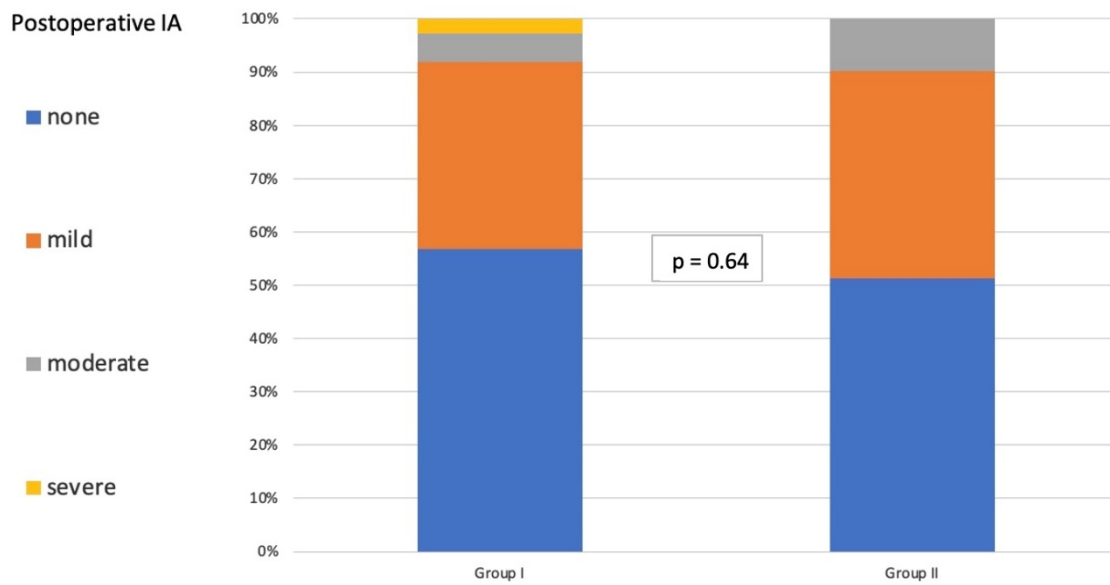


Figure S2. Postoperative aortic valve regurgitation (*P*-value Mann–Whitney test)

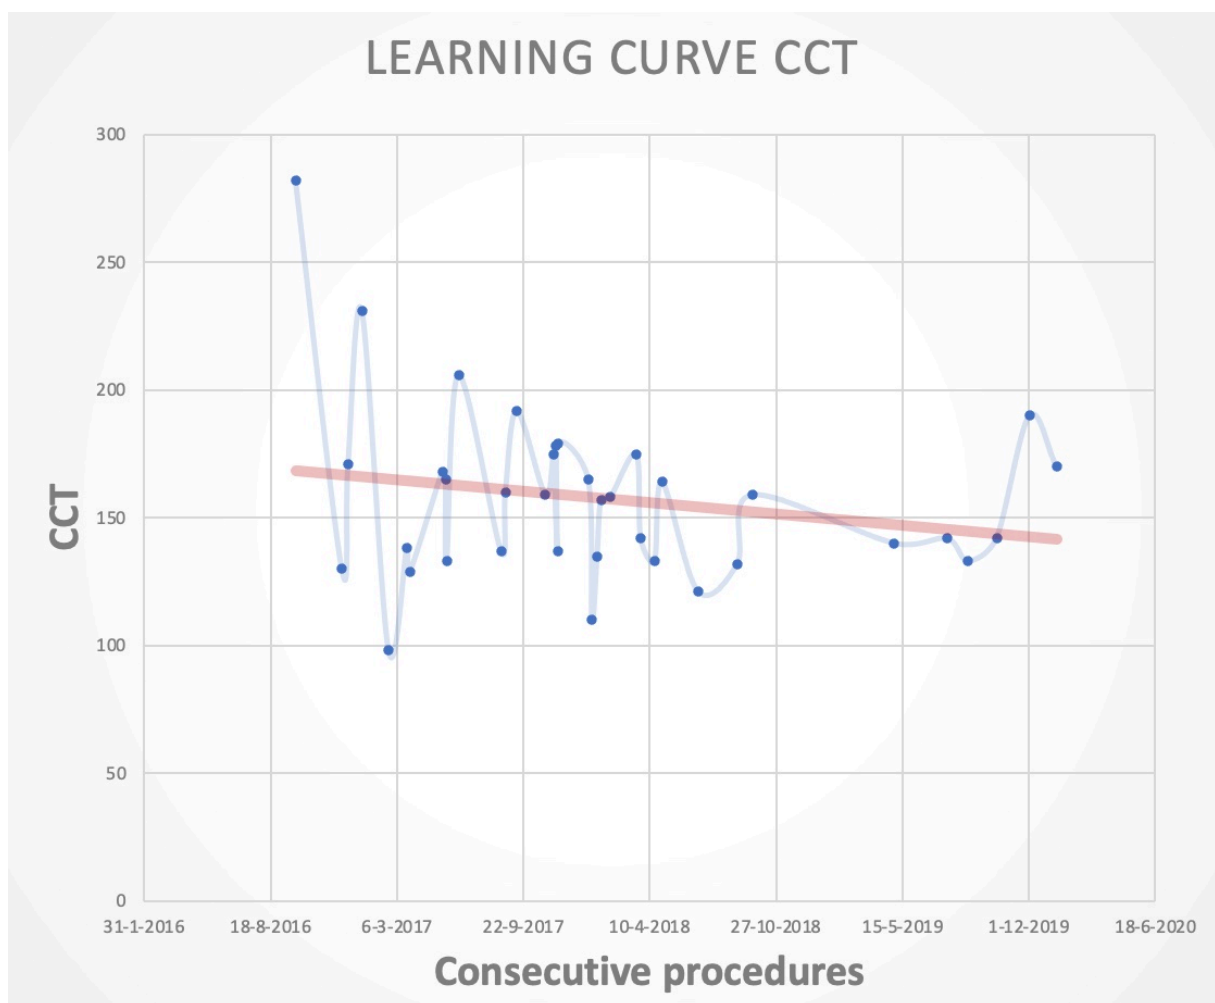


Figure S3. Learning curve — cross clamp time

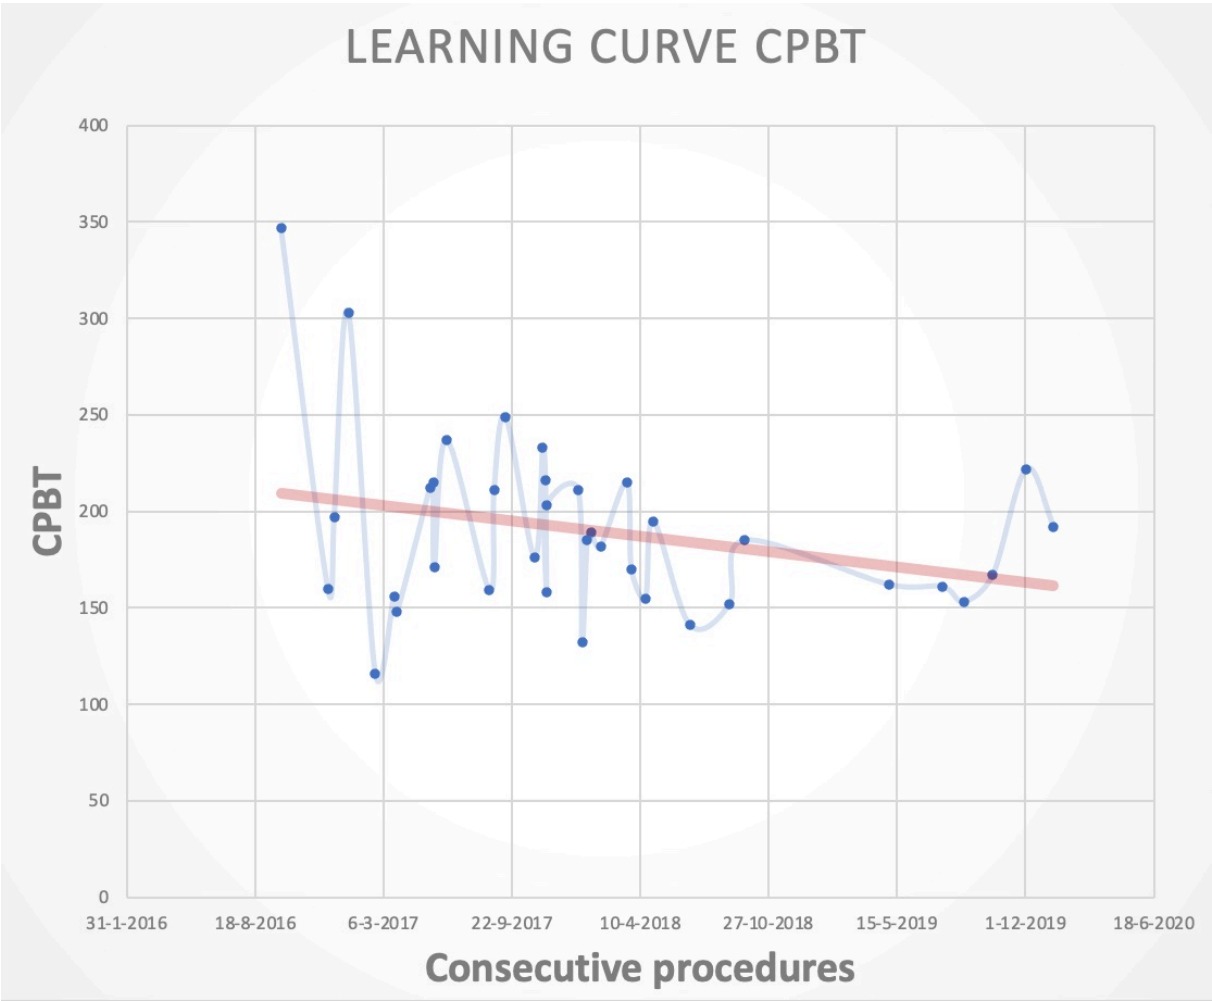


Figure S4. Learning curve — cardiopulmonary bypass time